

openheart First-generation versus second-generation drug-eluting stents in current clinical practice: updated evidence from a comprehensive meta-analysis of randomised clinical trials comprising 31 379 patients

Eliano Pio Navarese,^{1,2,13} Mariusz Kowalewski,^{3,13} David Kandzari,^{4,13} Alexandra Lansky,⁵ Bartosz Górny,^{3,13} Łukasz Kołtowski,^{6,13} Ron Waksman,⁷ Sergio Berti,^{1,13} Giuseppe Musumeci,^{8,13} Ugo Limbruno,⁹ Rene J van der Schaaf,¹⁰ Malte Kelm,^{2,13} Jacek Kubica,^{11,13} Harry Suryapranata¹²

To cite: Navarese EP, Kowalewski M, Kandzari D, *et al.* First-generation versus second-generation drug-eluting stents in current clinical practice: updated evidence from a comprehensive meta-analysis of randomised clinical trials comprising 31 379 patients. *Open Heart* 2014;**1**: e000064. doi:10.1136/openhrt-2014-000064

► Additional material is available. To view please visit the journal (<http://dx.doi.org/10.1136/openhrt-2014-000064>).

Received 18 February 2014

Revised 15 May 2014

Accepted 15 July 2014



CrossMark

For numbered affiliations see end of article.

Correspondence to

Dr Eliano Pio Navarese; eliano.navarese@alice.it

ABSTRACT

Background: First-generation drug-eluting stents (DES) have become the most widely used devices worldwide for management of coronary artery disease. As remote follow-up data were becoming available, concerns emerged in regard to their long-term safety. Second-generation DES were designed to overcome safety issues, but the results of randomised clinical trials remain conflicting.

Methods: We compared the safety and efficacy of first-generation versus second-generation Food and Drug Administration approved DES; the following devices were included: first-generation sirolimus-eluting stent (SES) and paclitaxel-eluting stents (PES); second-generation everolimus-eluting stent (EES), zotarolimus-eluting stent Endeavor and ZES-Resolute (ZES-R). Prespecified safety end points comprised ≤ 1 and >1 year: overall and cardiac mortality, myocardial infarction (MI), definite/definite or probable ST; efficacy end points were target lesion revascularisation and target vessel revascularisation. Composite end points were analysed as well.

Results: 33 randomised controlled trials involving 31 379 patients with stable coronary artery disease or acute coronary syndrome undergoing DES implantation were retrieved. No differences in mortality among devices were found. In the overall class comparison, second-generation DES were associated with a 22% reduction of odds of MI at short-term OR 0.77 (95% CI 0.68 to 0.89) $p=0.0002$; EES reduced the odds of definite-probable ST compared with PES: OR 0.33 (95% CI 0.15 to 0.73) $p=0.006$; First-generation SES along with second-generation EES and ZES-R showed similar efficacy in decreasing the odds of repeat revascularisation.

Conclusions: Second-generation EES and ZES-R offer similar levels of efficacy compared with first-generation SES, but are more effective than PES; however, only

KEY MESSAGES

What is already known about this subject?

- Second generation DES are similarly effective as first generation DES.

What does this study add?

- Everolimus eluting stent was found to significantly reduce the odds of myocardial infarction and stent thrombosis.

How might this impact on clinical practice?

- No differences in mortality was found between these devices.

second-generation EES significantly reduced the incidence of MI and ST, and therefore should be perceived as the safest DES to date.

INTRODUCTION

Over the past 10 years, first-generation drug-eluting stents (DES), especially sirolimus-eluting stent (SES) and paclitaxel-eluting stents (PES), have become the most widely used devices worldwide for management of coronary artery disease. However, despite their clear superiority in preventing restenosis and the need for repeat revascularisation due to eluted antiproliferative drugs is certainly proven,¹ as remote follow-up data were becoming available, concerns emerged in regard to their long-term safety, strictly late and very late thrombotic events, in turn associated with a high rate of death and

Table 1 Characteristics of included studies

Study	Journal	Year	Number of patients	First generation	Second generation	Short-term follow-up (≤12 months)	Long-term follow-up (>12 months)	Primary end point	MACE/TVF definition	Clinical setting	Minimal DAPT duration (ADP receptor/P2Y12 inhibitor)	Protocol defined follow-up angiography
APPENDIX-AMI ^{13 14}	<i>PLoS ONE</i>	2013	977	SES Cypher	EES Xience V	12 months*	24 months	MACE	Cardiac mortality, MI, TVR	Stable/ACS	12 months	No
BASKET-PROVE ¹⁵	<i>NEJM</i>	2010	1549	SES Cypher	EES Xience V	n.r.	24 months	MACE	Mortality, MI, TVR	Stable/ACS	12 months	No
CATOS ¹⁶	<i>Circulation Journal</i>	2012	160	SES Cypher	ZES Endeavor	12 months	n.r.	In-segment binary restenosis rate at 9 months angiographic follow-up	Cardiac mortality, MI, TVR	CTO	12 months	Yes
CIBELES ¹⁷	<i>Circulation Cardiovascular Interventions</i>	2013	207	SES Cypher	EES Xience V	12 months	n.r.	In-stent late loss at 9 months angiographic follow-up	Mortality, MI, TVR	TCO	12 months	Yes
COMPARE ^{18–20}	<i>Lancet</i>	2010	1800	PES Taxus Liberté	EES Xience V	12 months	24, 36 months	MACE	Mortality, MI, TVR	Stable/ACS	12 months	No
ENDEAVOR III ^{21 22}	<i>JACC Cardiovascular Interventions</i>	2006 2011	436	SES Cypher	ZES Endeavor	9 months	60 months	In-segment late lumen loss at 8 months angiographic follow-up	Mortality, MI, TLR	Stable/ACS	3 months	Yes
ENDEAVOR IV ^{23 24}	<i>JACC Cardiovascular Interventions</i>	2010 2013	1548	PES Taxus Express	ZES Endeavor	12 months	60 months	TVF at 9 months	Mortality, MI, TLR	Stable/ACS	6 months	Yes
ESSENCE-Diabetes ²⁵	<i>Circulation</i>	2011	300	SES Cypher	EES Xience V	12 months	n.r.	In-segment late lumen loss at 8 months angiographic follow-up	Mortality, MI, TLR	Stable/ACS	12 months	Yes
EXCELLENT ²⁶	<i>JACC</i>	2011	1428	SES Cypher	EES Xience V or Promus	12 months	n.r.	In-segment late lumen loss at 9 months angiographic follow-up	Cardiac mortality, MI, TLR	Stable/ACS	6 months	Yes
EXECUTIVE ²⁷	<i>JACC Cardiovascular Interventions</i>	2013	200	PES Taxus Liberté	EES Xience V	12 months	n.r.	In-segment late lumen loss at 9 months angiographic follow-up	Mortality, MI, TVR	Stable/ACS	6 months	Yes
ISAR-TEST-2 ^{28 29}	<i>EHJ JACC</i>	2009 2010	674	SES Cypher	ZES Endeavor	12 months	24 months	binary angiographic restenosis at 6–8-month follow-up angiography	Mortality, MI, TLR	Stable/ACS	12 months	Yes
KOMER ³⁰	<i>EuroIntervention</i>	2011	611	SES Cypher and PES Taxus Express	ZES Endeavor	12 months	18 months	MACE	Cardiac mortality, MI, TLR	STEMI	12 months	Yes

Continued

Table 1 Continued

Study	Journal	Year	Number of patients	First generation	Second generation	Short-term follow-up (≤12 months)	Long-term follow-up (>12 months)	Primary end point	MACE/TVF definition	Clinical setting	Minimal DAPT duration (ADP receptor/P2Y12 inhibitor)	Protocol defined follow-up angiography
LONG-DES III ³¹	JACC	2011	450	SES Cypher	EES Xience V or Promus	12 months	n.r.	In-segment late lumen loss at 9 months angiographic follow-up	Mortality, MI, TVR	Stable/ACS	12 months	Yes
LONG-DES IV ³²	<i>Circulation Cardiovascular Interventions</i>	2012	500	SES Cypher	ZES Resolute	12 months	n.r.	In-segment late lumen loss at 9 months angiographic follow-up	Mortality, MI, TVR	Stable/ACS	12 months	Yes
Naples-Diabetes ³³	<i>Circulation Cardiovascular Interventions</i>	2011	226	SES Cypher and PES Taxus Liberte	ZES Endeavor	In-hospital; 12 months	36 months	MACE	Mortality, MI, TVR	Stable/ACS	6 months	No
PRISON III ³⁴	<i>EuroIntervention</i>	2013	304	SES Cypher	ZES Resolute or ZES Endeavor	12 months	n.r.	In-segment late lumen loss at 8 months angiographic follow-up	Mortality, MI, TLR	TCO	12 months	Yes
R-CHINA RCT ³⁵	JACC <i>Cardiovascular Interventions</i>	2013	400	PES Taxus Liberte	ZES Resolute	12 months	n.r.	In-stent late lumen loss at 9 months angiographic follow-up	Mortality, MI, TLR	Stable/ACS	6 months	Yes
RESET ³⁶	<i>Circulation</i>	2012	3197	SES Cypher	EES Xience V	12 months	n.r.	TLR at 12 months; composite of all-cause death and MI at 36 months	Cardiac mortality, MI, TLR	Stable/ACS	3 months	No
Sakakibara et al ³⁷	<i>Circulation Journal</i>	2012	100	SES Cypher	EES Xience V	12 months	n.r.	binary angiographic restenosis at 8 month follow-up angiography	Mortality, MI, TLR	Stable	12 months	Yes
Sawada et al ³⁸	<i>International Journal of Cardiology</i>	2012	35	SES Cypher	EES Xience V or Promus	7 months	n.r.	Neointimal thickness and ST	n.a.	STEMI	7 months	Yes
SEA-SIDE ³⁹	JACC <i>Cardiovascular Interventions</i>	2011	150	SES Cypher	EES Xience V	n.r.	18 months	Occurrence of any trouble in the side-branch (SB) management	Mortality, MI, TVR	Stable/ACS	12 months	No
SEZE ⁴⁰	<i>Chinese Medical Journal</i>	2012	122	SES Cypher	ZES Endeavor	12 months	n.r.	In-stent late lumen loss at 9 months angiographic follow-up	Cardiac mortality, MI, TVR	STEMI	12 months	Yes
Song et al ⁴¹	JACC	2012	1114	SES Cypher	EES Xience V	12 months	n.r.	In-segment late lumen loss at 9 months angiographic follow-up	Mortality, MI, TVR	Stable/ACS	6 months	Yes

Continued

Table 1 Continued

Study	Journal	Year	Number of patients	First generation	Second generation	Short-term follow-up (≤12 months)	Long-term follow-up (>12 months)	Primary end point	MACE/TVF definition	Clinical setting	Minimal DAPT duration (ADP receptor/P2Y12 inhibitor)	Protocol defined follow-up angiography
SORT OUT III ^{42 43}	<i>Lancet JACC Cardiovascular Interventions</i>	2010 2013	2332	SES Cypher	ZES Endeavor	9 months	36 months	MACE	Cardiac mortality, MI, TVR	Stable/ACS	12 months	No
SORT OUT IV ^{44 45}	<i>Circulation JACC</i>	2012 2012	2774	SES Cypher	EES Xience V or Promus	9 months	24, 36 [ref-tctmd] months	MACE	Cardiac mortality, MI, TVR, def. ST	Stable/ACS	12 months	No
SPIRIT II ^{46 47}	<i>EuroIntervention EuroIntervention</i>	2007 2012	300	PES Taxus Liberte or PES Taxus Express	EES Xience V	12 months	60 months	In-stent late lumen loss at 6 months angiographic follow-up	Cardiac mortality, MI, TLR	Stable/ACS	12 months	Yes
SPIRIT III ^{48 49}	<i>JAMA The American Journal of Cardiology NEJM JACC</i>	2008 2011	1001	PES Taxus Express	EES Xience V	12 months	36, 60 [ref stone ppt] months	In-stent late lumen loss at 8 months angiographic follow-up	Cardiac mortality, MI, TLR	Stable/ACS	6 months	Yes
SPIRIT IV ^{50 51}	<i>NEJM JACC</i>	2010 2011	3687	PES Taxus Express	EES Xience V	12 months	24 months	Composite of cardiac death, target vessel MI and TLR	Cardiac mortality, MI, TLR	Stable/ACS	12 months	No
SPIRIT V Diabetic Study ⁵²	<i>American Heart Journal</i>	2012	324	PES Taxus Liberte	EES Xience V	12 months	n.r.	In-stent late lumen loss at 9 months angiographic follow-up	Cardiac mortality, MI, TVR	Stable/ACS	6 months	Yes
Wang et al ⁵³	<i>JACC abstracts</i>	2011	875	SES Cypher	ZES Endeavor	6 months	n.r.	MACE	Cardiac mortality, MI, TLR	STEMI	n.r.	No
XAMI ⁵⁴	<i>JACC</i>	2012	625	SES Cypher	EES Xience V	12 months	n.r.	MACE	Cardiac mortality, MI, TVR	STEMI	12 months	No
ZEST ⁵⁵	<i>JACC</i>	2010	2645	SES Cypher or PES Taxus Liberte	ZES Endeavor	12 months	n.r.	MACE	Mortality, MI, TVR	Stable/ACS	12 months	Yes
ZEST-AMI ^{56 57}	<i>The American Journal of Cardiology</i>	2009	328	SES Cypher or PES Taxus Liberte	ZES Endeavor	12 months	n.r.	MACE	Mortality, MI, TVR	STEMI	12 months	Yes

ACS, acute coronary syndrome; DAPT, dual antiplatelet therapy; EES, everolimus-eluting stent; MACE, major adverse cardiovascular events; MI, myocardial infarction; PES, paclitaxel-eluting stent; SES, sirolimus-eluting stent; STEMI, ST elevation myocardial infarction; TLR, target lesion revascularisation; TVR, target vessel revascularisation; ZES, zotarolimus-eluting stent.

myocardial infarction (MI).^{2, 3} Such events have been attributed to the incomplete re-endothelialisation caused by the drug-induced inhibition of endothelial cell proliferation, stent malapposition, accelerated neoatherosclerosis and, importantly, polymer-induced prolonged vessel wall inflammation.⁴ Second-generation DES were designed to overcome safety issues in the long term, employing new biocompatible polymer coatings, less toxic antiproliferative drugs and eventually state-of-the-art thin strut Co-Cr metal alloys, and extensively tested in randomised clinical trials (RCTs). The everolimus-eluting stent (EES) has been found to be safer than first-generation and biodegradable DES;⁵ on the other hand, zotarolimus-eluting stent (ZES) was inferior to SES in terms of major adverse cardiac events (MACE) and superior to PES in terms of MI in independent recent meta-analyses of RCTs.^{6, 7}

Driven by conflicting evidence on first-generation versus second-generation DES performance in regard to efficacy and safety along with another recent meta-analysis⁸ showing significant outcomes in one comparison only (ST rates reduction with second-generation EES vs first-generation PES, we performed a comprehensive and updated meta-analysis of all relevant DES data published to date comparing first-generation and second-generation DES in clinical practice.

METHODS

We compared the safety and efficacy of first-generation vs second-generation Food and Drug Administration (FDA) approved DES; the following devices were included: first-generation SES and PES, 2) second-generation EES, ZES-Endeavor (ZES-E) and ZES-Resolute (ZES-R).

Established methods were used in adherence to the Preferred Reporting Items for Systematic reviews and Meta-Analyses (PRISMA) statement for reporting systematic reviews and meta-analyses in healthcare interventions.⁹ Relevant RCTs were searched until September 2013 through MEDLINE, the Cochrane Central Register of Controlled Trials (CENTRAL), Google Scholar and EMBASE databases and through <http://www.tctmd.com>, <http://www.clinicaltrials.gov>, <http://www.clinicaltrialresults.org> and <http://www.cardiosource.com> websites; documents accessible through the FDA website were scrutinised as well. The following keywords were used: “randomized trials”, “drug-eluting stent”, “durable polymer stent”, “sirolimus stent”, “paclitaxel stent”, “everolimus stent”, “zotarolimus stent”, “Endeavor zotarolimus-stent”, “Resolute zotarolimus-stent”. No language, date or publication status restrictions were imposed. For each RCT, the most updated or most inclusive data were used.

Citations were screened at the title/abstract level and retrieved as full reports. Inclusion criteria were: (1)

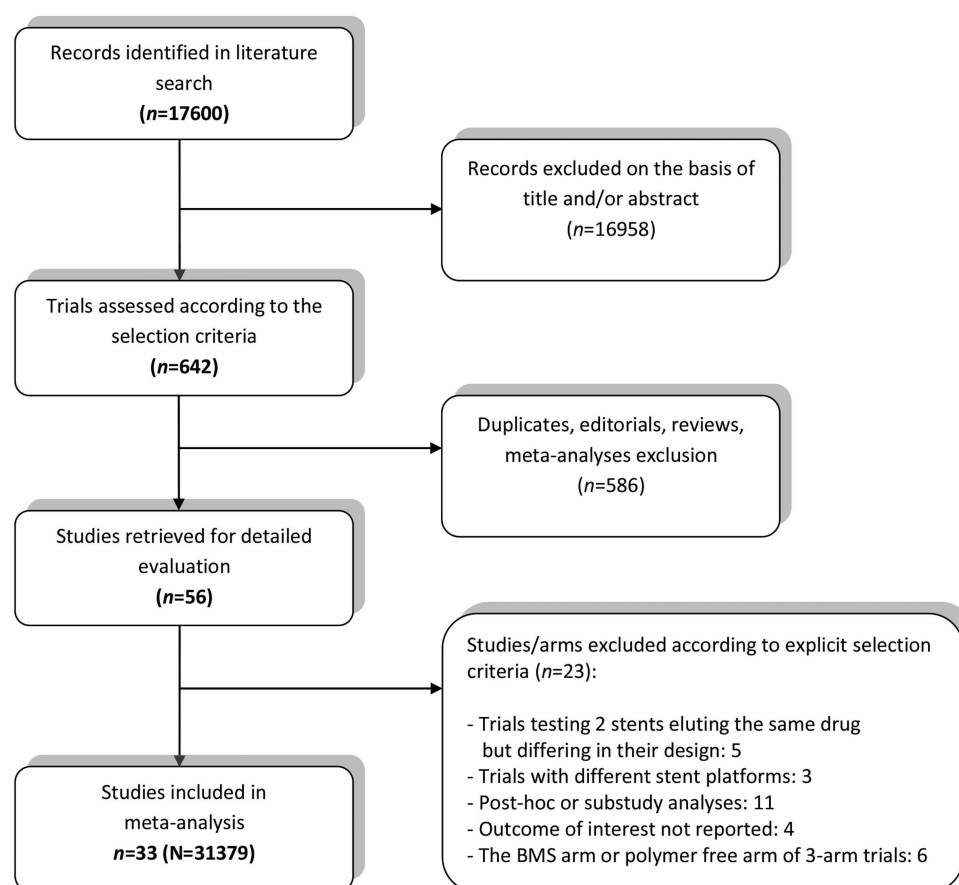


Figure 1 Flow diagram of the review process according to the Preferred Reporting Items for Systematic reviews and Meta-Analyses (PRISMA) statement.




Figure 2 Analysis of all-cause mortality at short-term (A) and long-term (B) follow-up. ORs and 95% CIs. Size of squares is proportional to the statistical weight of each trial.

human studies; (2) RCTs; (3) studies comparing safety AND/OR efficacy of first-generation versus second-generation durable polymer DES; (4) additional data from retrieved studies available at a longer follow-up. Exclusion criteria were: (1) non-RCTs; (2) a substudy of RCTs; (3) a bare metal stent (BMS), biodegradable/bioabsorbable stent or polymer-free stent as the control group, (4) RCTs comparing DES within their class.

Internal validity was appraised according to the proper allocation sequence/concealment, patient blinding, investigator blinding and complete outcome data/full reporting.

Prespecified safety end points comprised ≤ 1 year: overall and cardiac mortality, MI and definite/definite or probable ST according to the definition criteria of the Academic Research Consortium (ARC).¹⁰ Efficacy




Figure 2 Continued

end points were target lesion revascularisation (TLR) and target vessel revascularisation (TVR). We also analysed the composite end point of MACE to appreciate the cumulative effect of combining non-frequent safety and efficacy adverse events; the MACE definition of each individual study was accepted, although it varied across studies (table 1). To account for over time changes in both the DES properties and eluted drug release kinetics, analyses of each clinical outcome were repeated at longest available, beyond 1 year follow-up.

Statistical analysis

Data were analysed according to the intention-to-treat principle. ORs and 95% CIs were used as summary statistics. Heterogeneity was assessed by the Cochran Q test. Statistical heterogeneity was summarised by the I^2 statistic, which quantifies the percentage of variation in study results that is due to heterogeneity rather than chance.¹¹ Pooled ORs were calculated using a fixed effect model with the Mantel-Haenszel method. The random effects model was applied in case of significant heterogeneity and/or moderate or significant inconsistency (heterogeneity $>50\%$; inconsistency $p \leq 0.05$) across studies.¹² Results were considered statistically significant at two-sided $p \leq 0.05$. All pooling analyses were conducted using Review Manager 5.1 (Cochrane Collaboration, Copenhagen, Denmark).

RESULTS

Studies and patient population

The PRISMA flow diagram of the studies selection is presented in figure 1. The full electronic MEDLINE database search process along with inclusion/exclusion criteria and risk of bias analysis of included studies is shown in the online supplementary material. Thirty-three^{13–57} trials comprising a total of 31 379 patients met the inclusion criteria and entered the analysis. Information on stent comparators, clinical setting, minimal DAPT duration and primary end points is delineated in table 1. Most trials enrolled high-risk patients with stable coronary artery disease and acute coronary syndrome presentations, with six trials restricting their inclusion criteria to STEMI patients only^{30 38 40 53 54 56}; clopidogrel was administered across all studies; the composite end point of MACE was similar throughout the studies and included cardiac death, MI and repeat revascularisation; detailed definitions are listed in table 1. Funnel plots did not reveal publication bias or small study effect and are included in the online supplementary material (see online supplementary figure S1A, B).

Mortality, cardiac death

Twenty-nine studies contributed to the analysis of ≤ 1 year mortality. Second-generation DES were associated with results that did not differ significantly from

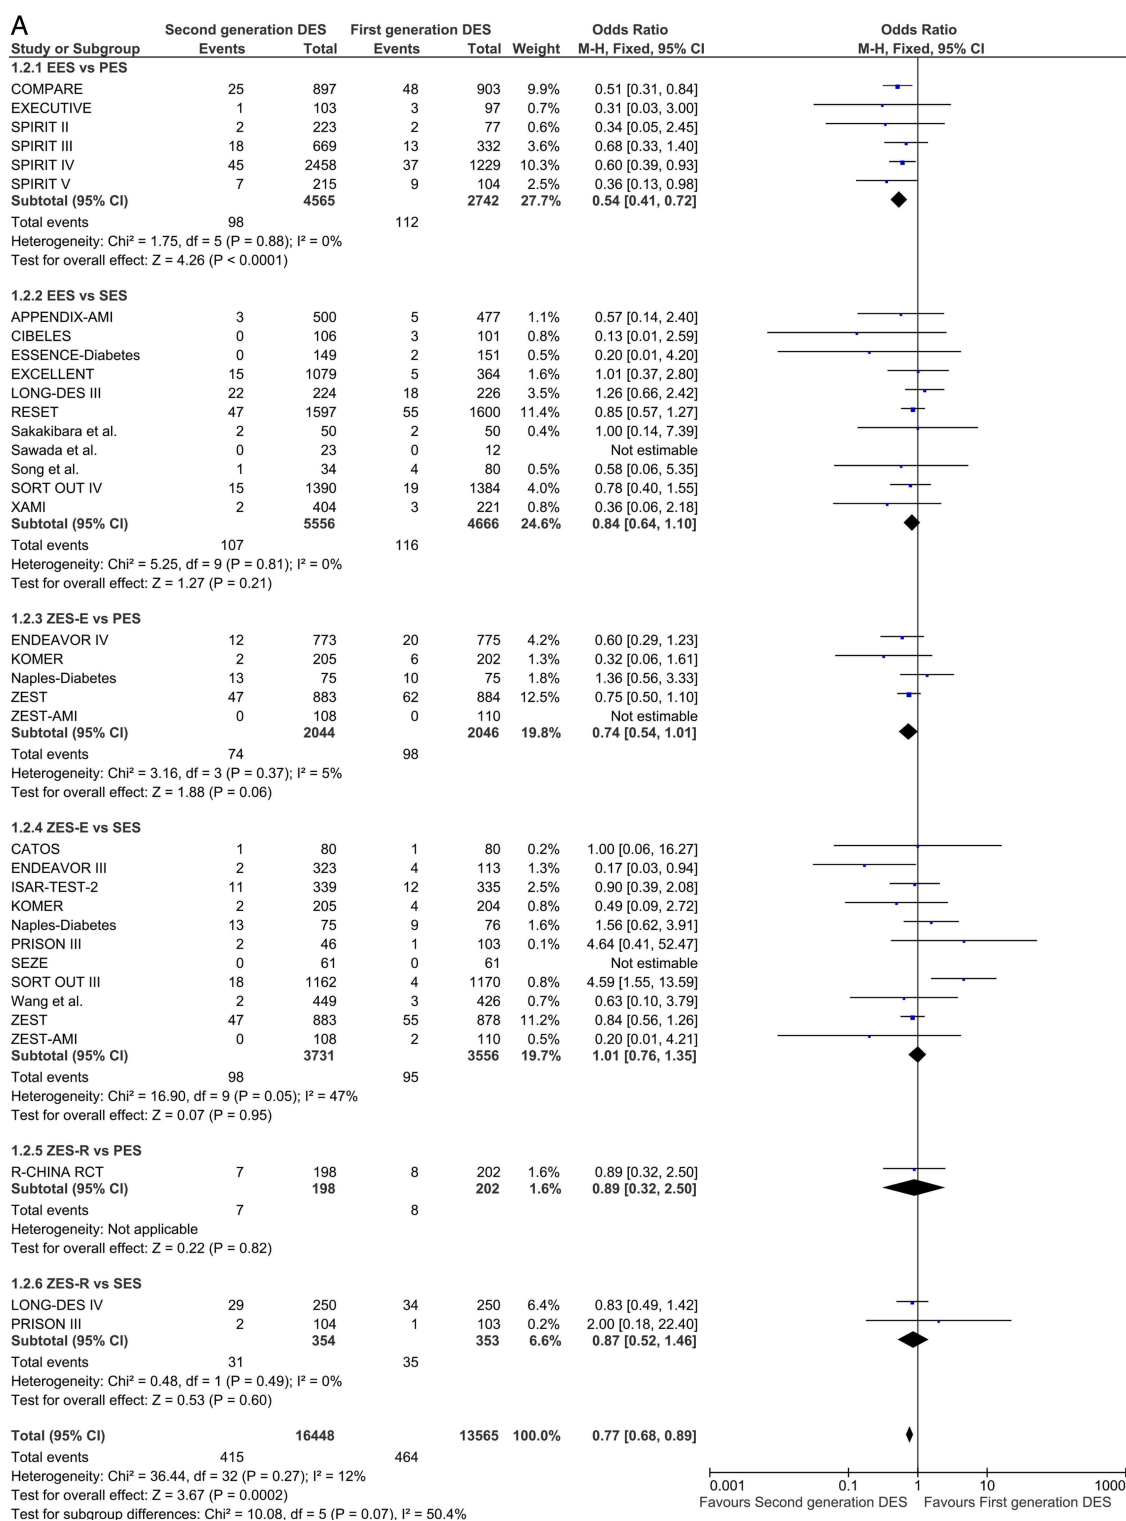


Figure 3 Analysis of MI at short-term (A) and long-term (B) follow-up. ORs and 95% CIs. Size of squares is proportional to the statistical weight of each trial. MI, myocardial infarction.

those of the first-generation in either comparison group: OR 0.99 (95% CI 0.81 to 1.20) $p=0.90$. Results in the long term (13 studies included) were consistent with the short-term analysis: OR 0.94 (95% CI 0.77 to 1.16) $p=0.58$ (figure 2A). A non-significant trend favouring EES was shown in comparison with PES in the long term: OR 0.68 (95% CI 0.43 to 1.09) $p=0.06$ (figure 2B).

The cardiac mortality analysis did not diverge from the findings from all-cause death calculations with OR 1.03 (95% CI 0.81 to 1.31) $p=0.79$ and OR 1.02 (95% CI 0.79 to 1.31) $p=0.89$, for short-term and long-term follow-up, respectively, for overall first-generation versus second-generation stents comparison (see online supplementary figure S2A,B).




Figure 3 Continued

Myocardial infarction

Thirty-one studies were included in the MI analysis in the short term. EES significantly reduced the odds of MI compared with PES: OR 0.54 (95% CI 0.41 to 0.72) $p < 0.0001$ (figure 3A). In the overall class comparison, second-generation DES were associated with a 23% reduction of odds of MI OR 0.77 (95% CI 0.68 to 0.89) $p = 0.0002$ in the short term. A significant class effect favouring second-generation DES was sustained in the long-term analysis: OR 0.75 (95% CI 0.56 to 1.00) $p = 0.05$, with the odds of MI halved in comparison with EES versus PES: OR 0.56 (95% CI 0.44 to 0.72) $p < 0.001$ (figure 3B).

Stent thrombosis

For the analysis of definite ST, 26 studies were included. In the short term, EES was associated with significant reduction of odds of ST compared with PES and SES: OR 0.34 (95% CI 0.18 to 0.62) $p = 0.0005$ and OR 0.43 (95% CI 0.22 to 0.84) $p = 0.01$, respectively (figure 4A). Second-generation ZES-E increased the odds of ST by 122% compared with first-generation SES: OR 2.22 (95% CI 1.14 to 4.31) $p = 0.02$. Results in the long term confirmed short follow-up findings; EES was associated with a more pronounced and significant reduction of odds of ST over time as compared with PES and SES:

OR 0.26 (95% CI 0.14 to 0.49) $p < 0.0001$ and OR 0.30 (95% CI 0.11 to 0.78) $p = 0.01$, respectively (figure 4B).

Analysis of definite-probable ST reflected the direction of the definite ST estimates. EES reduced the odds of definite-probable ST compared with PES and SES: OR 0.33 (95% CI 0.15 to 0.73) $p = 0.006$ and OR 0.61 (95% CI 0.37 to 1.01) $p = 0.05$ (see online supplementary figure 3A). Also, at long-term follow-up, a significant reduction of definite-probable ST odds was observed with EES versus PES (OR 0.32 (95% CI 0.17 to 0.59) $p = 0.0002$) and versus SES (OR 0.50 (95% CI 0.28 to 0.88) $p = 0.02$; see online supplementary figure 3B). The overall class comparison of definite-probable ST favoured second-generation DES over SES at both short-term (OR 0.67 (95% CI 0.47 to 0.94) $p = 0.02$) and long-term (OR 0.54 (95% CI 0.37 to 0.80) $p = 0.002$) follow-up.

Repeat revascularisation TLR/TVR

Twenty-nine studies reported TLR incidence at short-term follow-up. First-generation SES along with second-generation EES and ZES-R showed a similar degree of efficacy in decreasing the odds of TLR. EES reduced the odds of TLR by 43% compared with PES (OR 0.57 (95% CI 0.36 to 0.91) $p = 0.02$) and ZES-E markedly increased the odds in comparison to SES (OR 2.61 (95% CI 1.97 to 3.46) $p < 0.00001$; figure 5A), with direction and significance of the estimates being sustained

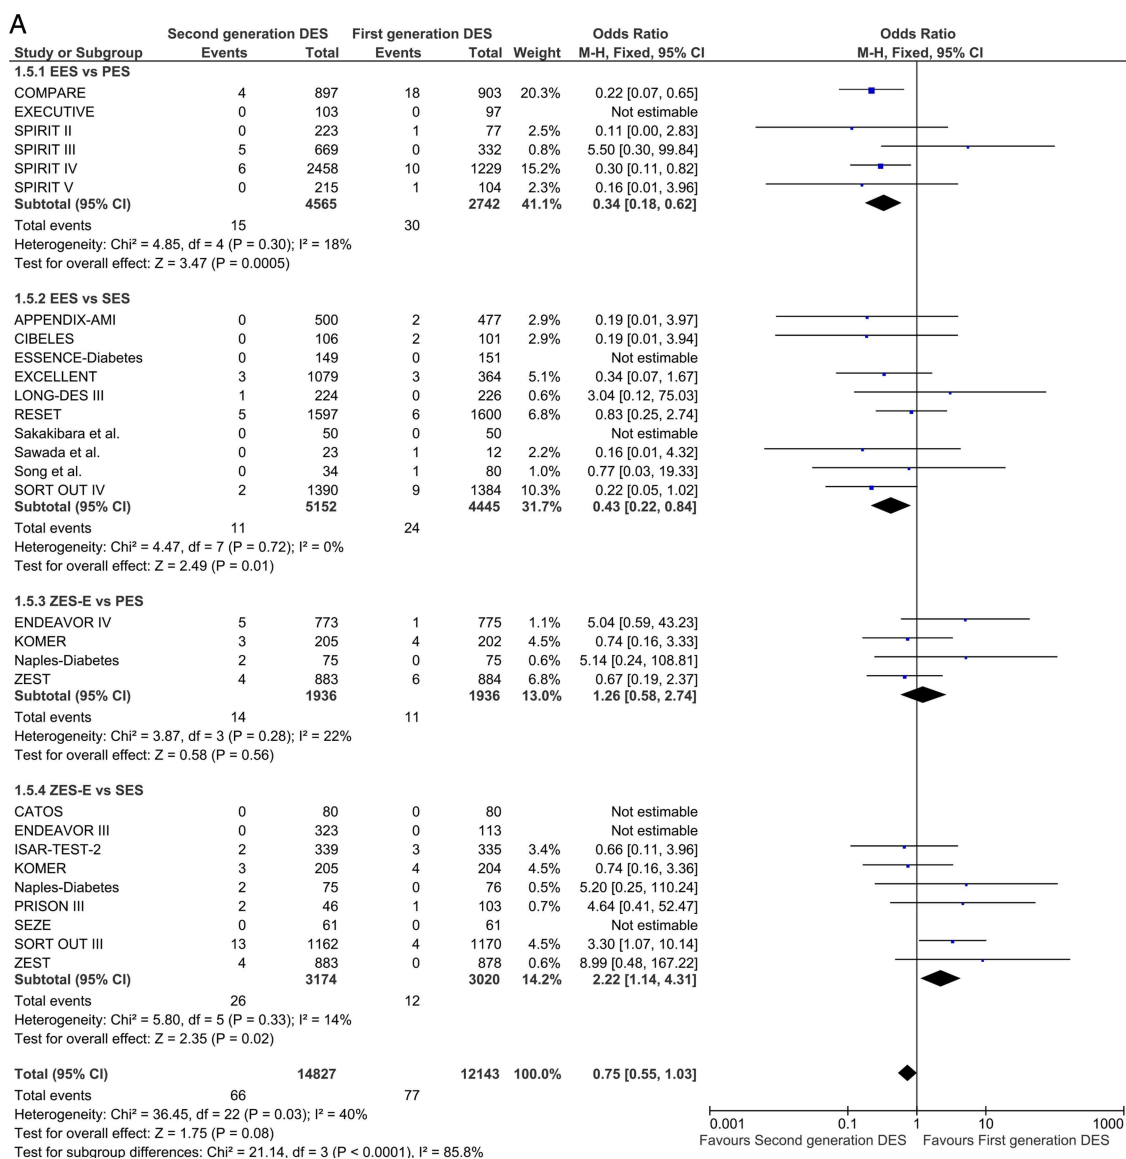


Figure 4 Analysis of definite ST at short-term (A) and long-term (B) follow-up. ORs and 95% CIs. Size of squares is proportional to the statistical weight of each trial. ST, stent thrombosis.

over long-term follow-up (12 studies; EES vs PES: OR 0.57 (95% CI 0.46 to 0.72) $p < 0.00001$; and ZES-E vs SES: OR 1.85 (95% CI 1.18 to 2.89) $p = 0.007$; figure 5B).

TVR calculations were in line with those of TLR, confirming a similar high efficacy of EES, SES and ZES-R but not ZES-E or PES at both short-term and long-term follow-up (see online supplementary figure S4A,B).

Major adverse cardiac events

The analysis of composite end point of MACE included 31 studies at short-term and 13 at long-term follow-up. EES and ZES-R were found to be significantly superior to PES (OR 0.63 (95% CI 0.52 to 0.76) $p < 0.00001$ and OR 0.44 (95% CI 0.21 to 0.92) $p = 0.03$) and ZES-E performed significantly worse than SES (OR 1.41 (95% CI 1.13 to 1.76) $p = 0.002$) in reducing the odds of MACE at ≤ 1 year (figure 6A). Long-term follow-up confirmed the direction and magnitude of the estimates with

EES reducing the odds of MACE by 37% compared with PES (OR 0.63 (95% CI 0.54 to 0.73) $p < 0.00001$; figure 6B).

Sensitivity analyses

Prespecified sensitivity analyses after exclusion of studies which did not mandate 12-month DAPT for the outcomes of MI and ST did not change the magnitude or direction of the estimates.

Myocardial infarction

Twenty-one studies were included in MI analysis in the short term. EES significantly reduced the odds of MI compared with PES: OR 0.55 (95% CI 0.40 to 0.76) $p = 0.0003$. In the overall class comparison, second-generation DES were associated with a 23% reduction of odds of MI OR 0.77 (95% CI 0.65 to 0.91) $p = 0.002$ in the short term. A borderline significant class effect favouring




Figure 4 Continued

second-generation DES was sustained in the long-term analysis: OR 0.75 (95% CI 0.55 to 1.01) $p=0.06$, with odds of MI roughly halved in comparison with EES versus PES: OR 0.56 (95% CI 0.42 to 0.74) $p<0.0001$.

Stent thrombosis

For the analysis of definite ST, 17 studies were included. In the short term, EES was associated with a significant reduction of odds of ST compared with PES and SES: OR 0.24 (95% CI 0.12 to 0.50) $p=0.0001$ and OR 0.46 (95% CI 0.21 to 0.99) $p=0.05$, respectively. Second-generation ZES-E increased the odds of ST by 122% compared with first-generation SES: OR 2.10 (95% CI 1.06 to 4.16) $p=0.03$. Results in the long term confirmed the short-term follow-up findings; EES was associated with a more pronounced and significant reduction of odds of ST over time as compared with PES and SES: OR 0.20 (95% CI 0.08 to 0.49) $p=0.0004$ and OR 0.30 (95% CI 0.12 to 0.75) $p=0.01$, respectively.

DISCUSSION

The present study is the largest report so far comparing first-generation versus second-generation DES. With 31 379 patients included, it provides the most comprehensive overview on the safety and efficacy outcomes of different first-generation and second-generation stents. The main findings of this meta-analysis are as follows:

(1) second-generation EES and ZES significantly reduced the incidence of MI compared with first-generation PES; (2) only second-generation EES significantly reduced the odds of definite and definite/probable ST compared with first-generation DES (3) second-generation EES and ZES-R, and the first-generation SES, are similar to each other with regard to their efficacy and significantly better than ZES-E and PES with regard to repeat coronary revascularisations.

In the present large-scale study analysis, single and composite safety end points did not differ in direction or magnitude of the effect favouring durable polymer EES.

Safety

First-generation DES have been found to be superior to BMS in reducing restenosis and the need for repeat revascularisation. Their performance in terms of safety, and strictly, increased propensity for late and very late thrombotic events, however, was questioned as long follow-up data were becoming available; further studies showed that late and very late stent thrombosis could be attributed to numerous complex mechanisms with device design-related factors being of paramount importance.⁴ The inflammation induced by the durable polymers of first-generation DES may result in delayed healing and incomplete covering of stent struts by new and functional endothelium, with uncovered stent struts serving as a source

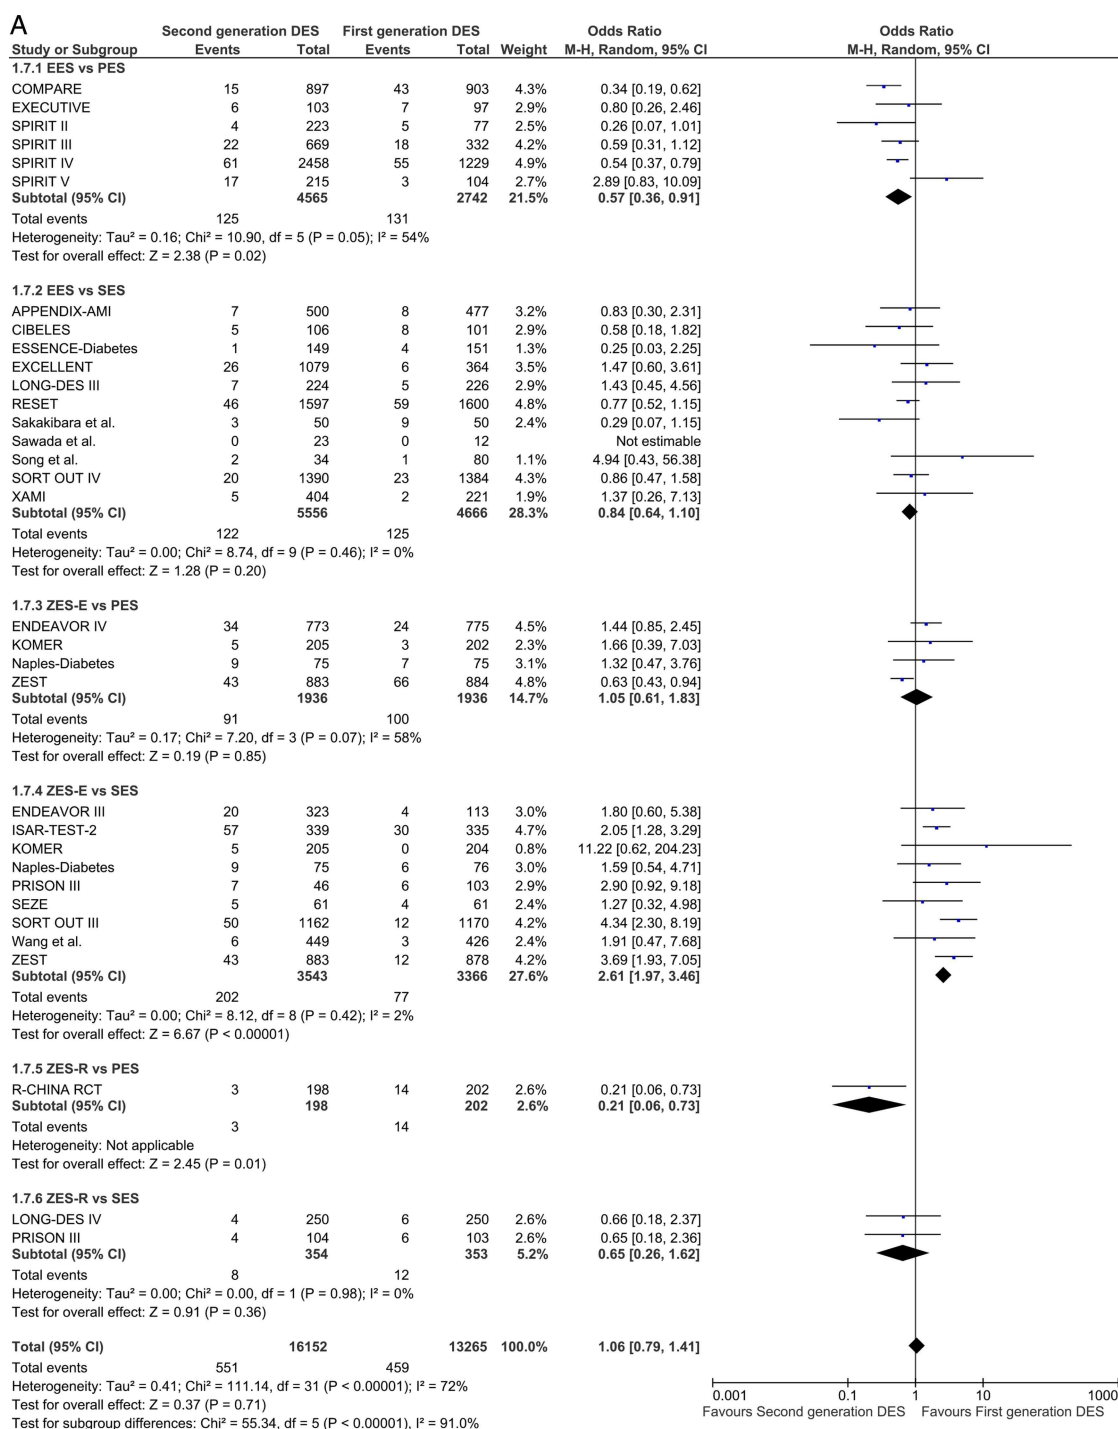


Figure 5 Analysis of TLR at short-term (A) and long-term (B) follow-up. ORs and 95% CIs. Size of squares is proportional to the statistical weight of each trial. TLR, target lesion revascularisation.

for future episodes of ST; second, other factors such as stent malapposition, mechanical tissue injury caused by stent struts during implantation and finally, polymer hypersensitivity or even toxicity, as is the case for PES,⁵⁸ in turn associated with persistent fibrin deposition, might also play a potential role. Second-generation DES were introduced to address the concerns raised by first generation DES by either optimising their metallic stent

platform or polymer and eluted drug; that is, second-generation EES uses thin struts coated with durable, fluorinated polymer, which has been shown to have thromboresistant properties in experimental studies; similarly, ZES-R combined more rapid elution kinetics than sirolimus (SES) in the same time offering thinner, more biocompatible phosphorylcholine polymer placed on a cobalt alloy stent platform.⁷




Figure 5 Continued

In the present meta-analysis, which compared most robust evidence of first-generation versus second-generation DES data, second-generation EES was found to be superior in regard to safety end points as compared with first-generation PES but not SES; this might be attributed to the proven overdose and/or accumulation of paclitaxel in the arterial wall due to a coronary uptake, in turn leading to toxicity, inflammation and late in-stent stenosis, which is not the case with SES.⁵⁹ The superiority of thin strut EES and ZES in reducing the incidence of MI in the short clinical follow-up might also come from mechanistic reasons; indeed, this might be related to the more frequent side branch jailing with thick strut devices (SES Cypher 140 μ m and PES Taxus Express 134 μ m vs ZES Endeavor/Resolute 91 μ m and Abbott Xience V 81 μ m), resulting in turn in higher rates of periprocedural MI.^{60–62} Although ST should be considered a surrogate safety end point, which must be interpreted in perspective of MI and mortality, it remains a devastating complication and is often associated with high rates of mortality and morbidity. Second-generation EES was associated with significantly lower rates of definite and definite or probable ST in short-term analysis compared with first-generation DES; this finding is in line with a meta-analysis by Palmerini,⁵ which for the first time demonstrated the superiority of EES over BMS and first-generation and second-generation DES in reducing early (0–30 days) and late

(31 days–12 months) ST. This analysis integrates the most updated data and enriches the previous findings of longer follow-up clinical data for particular devices, demonstrating for the first time that EES reduces definite and definite or probable ST also beyond these time frames (very late ST) compared with first-generation DES. Notably, data on EES do not reflect the performance of second-generation ZES-E in terms of stent thrombosis; indeed, Endeavor was found to even increase the incidence of definite ST as compared with SES at ≤ 1 year, mainly driven by the results of the SORT OUT III⁴² and ZEST⁵⁵ trials. As zotarolimus is a synthetic analogue of sirolimus, the disparities between stents are attributed to different kinetics of drug release from the polymers used for drug elution (1 week with ZES and 3 months with SES); postulated quick zotarolimus release and high initial concentrations not only affect the healing of the plaque and arterial wall, but may also allow for exposure of the atheromatous debris to the bloodstream, thus increasing the risk of early ST, which is of particular importance in high-risk patients with acute coronary syndrome or multivessel disease.

Efficacy and MACE

Design-related factors such as strut thickness, type of anti-proliferative agent, drug elution kinetics, elution time and type of polymer are all factors that may as well impact

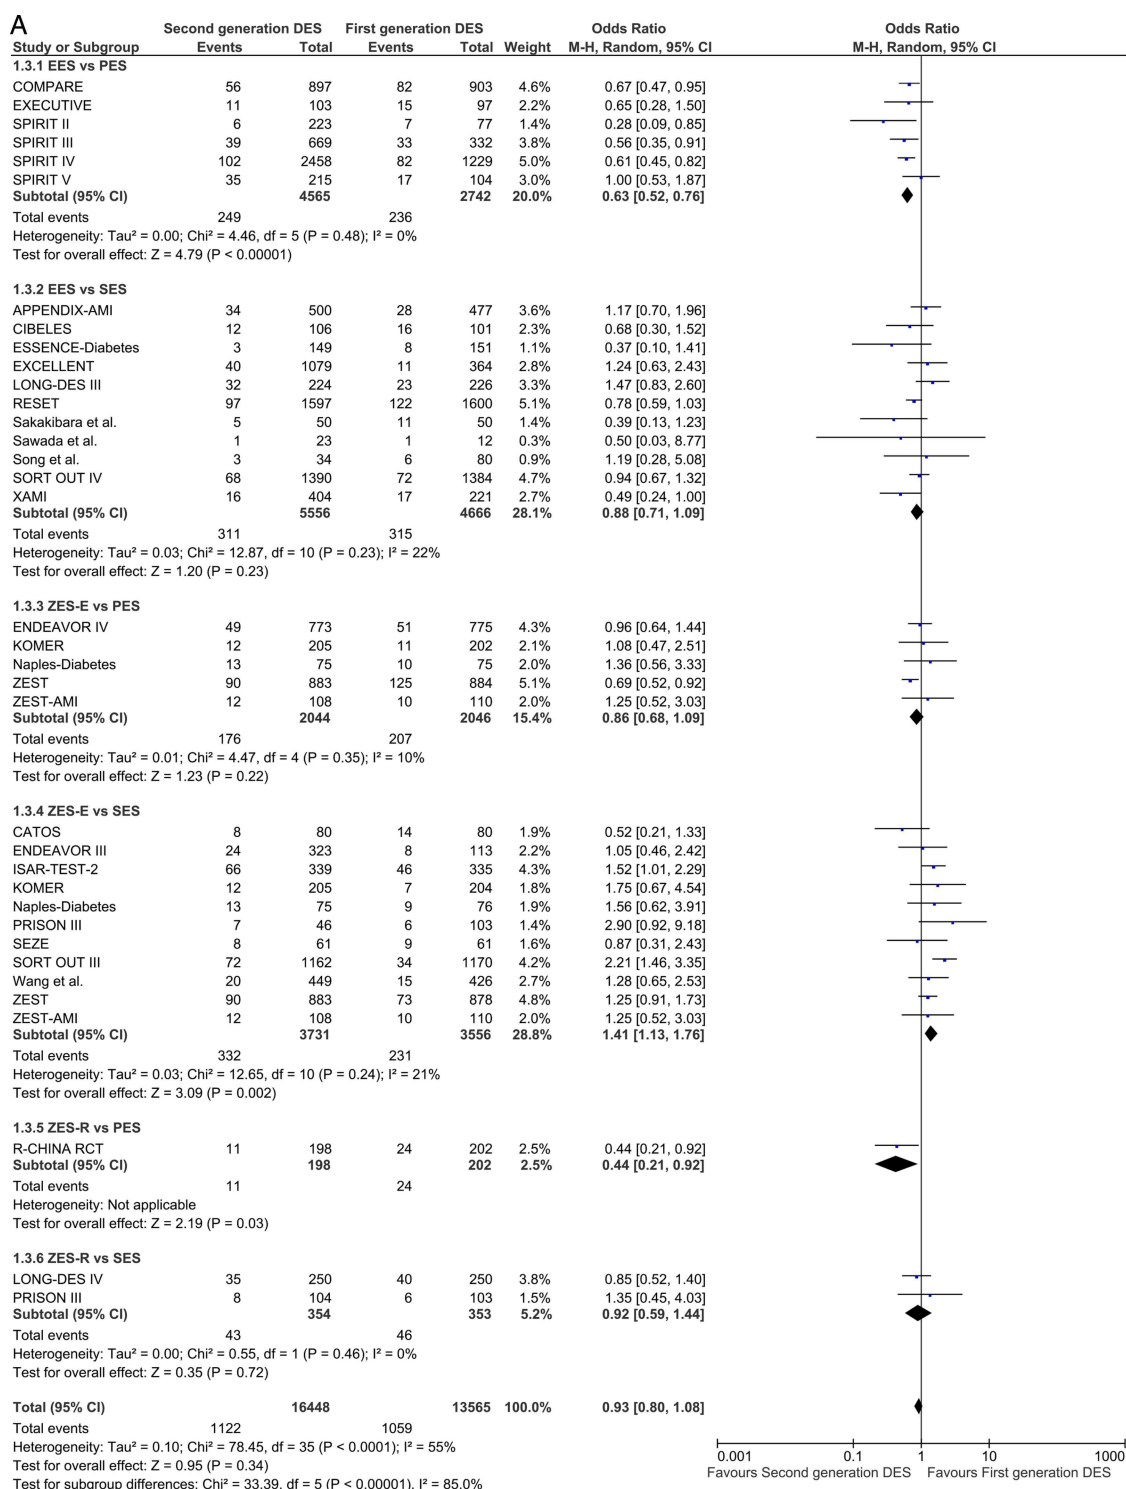


Figure 6 Analysis of MACE at short-term (A) and long-term (B) follow-up. ORs and 95% CIs. Size of squares is proportional to the statistical weight of each trial. MACE, major adverse cardiovascular events.

efficacy outcomes⁶³; although not a new finding, in this analysis all limus-eluting DES, with the exception of ZES-E, were associated with significantly lower rates of TLR/TVR than the first-generation PES. Taken together, inflammation causing properties of paclitaxel along with the short release curve of ZES-E preclude optimal suppression of procedure related injury responses, in turn resulting in subsequent intimal hyperplasia and increased

need for repeat revascularisation.⁶⁴ Unlike ZES-E, the more recently introduced ZES-R, which has a much longer (up to 180 days) release curve of the same antiproliferative agent, zotarolimus, is associated with a significant reduction in TVR/TLR compared with ZES-E.⁶⁵

In the present paper, we additionally analysed the incidence of MACE, which to the best of our knowledge is the most proper measure of device performance, as it




Figure 6 Continued

takes into account both safety and efficacy outcomes, providing statistical power given the low numbers of single outcome events. Not surprisingly, MACE analysis confirmed the single-outcome findings, with second-generation EES outperforming first-generation PES at ≤ 1 year and beyond. Remarkably, the initial short-term benefit of SES over ZES-E, attributable mainly to higher rates of repeat revascularisation with the latter, becomes less pronounced at long-term follow-up when drug elution is over.

Limitations

As with any meta-analysis, our study shares the limitations of the original studies. Results were analysed on trial level data, and therefore we could not assess whether all baseline characteristics were balanced among groups (although for the most part they were balanced within each RCT). Data for follow-ups longer than 1 year are limited but appear to confirm the direction of the estimates at ≤ 1 -year. The patient inclusion criteria of this meta-analysis are broad, more closely reflecting current practice, comprising stable and unstable high-risk patients. Potentially heterogeneous definitions of MI used across the trials may represent another limitation.

Another aspect is the duration of dual antiplatelet therapy (DAPT), that is, the combination of aspirin and

a P2Y₁₂ receptor blocker, which varied among the different trials. The variability of DAPT may, however, be less important in the context of the present meta-analysis given that BMS were excluded and most trials employed at least 6 months DAPT duration. Owing to the limited number of trials comparing ZES-R to first-generation DES, the findings with this device should be viewed as exploratory but certainly deserve further attention. Despite these limitations, this meta-analysis provides the largest-scale comparative information on the efficacy and safety profiles of different DES in current clinical practice.

CONCLUSIONS

Second-generation EES and ZES-R offer a similar level of efficacy compared with first-generation SES, but are more effective than PES; however, only second-generation EES significantly reduced the incidence of both MI and ST and therefore should be perceived as the safest DES to date.

Author affiliations

¹Invasive Cardiology, National Research Council Institute of Clinical Physiology (CNR-IFC), Pisa, Italy

²Department of Internal Medicine, Division of Cardiology, Pulmonology and Vascular Medicine, Heinrich-Heine-University, Düsseldorf, Germany

³10th Military Research Hospital and Polyclinic, Bydgoszcz, Poland

⁴Piedmont Heart Institute, Atlanta, Georgia, USA

⁵Department of Cardiology, Yale Medical School, New Haven, Connecticut, USA

⁶1st Department of Cardiology, Teaching Hospital, Medical University of Warsaw, Warsaw, Poland

⁷Division of Cardiology, MedStar Washington Hospital Center, Washington DC, USA

⁸Department of Cardiology, Ospedali Riuniti di Bergamo, Bergamo, Italy

⁹Department of Cardiology, Ospedale della Misericordia, Grosseto, Italy

¹⁰Department of Cardiology, Onze Lieve Vrouwe Gasthuis, Amsterdam, The Netherlands

¹¹Department of Cardiology and Internal Medicine, Ludwik Rydygier Collegium Medicum, Nicolaus Copernicus University, Bydgoszcz, Poland

¹²Department of Cardiology, Radboud University Nijmegen Medical Center, Nijmegen, The Netherlands

¹³Systematic Investigation and Research on Interventions and Outcomes (SIRIO) MEDICINE Research Network

Contributors All authors contributed to the present article. MK, BG and LK were responsible for data search and abstraction and critical analysis of eligibility. EPN and MK drafted the manuscript. DK, AL, RW, SB, GM, UL, RJvS, JK, and HS critically revised the manuscript.

Competing interests DK has received research/grant support from Boston Scientific, Medtronic, and Abbott Vascular and has served as consultant for Boston Scientific, Medtronic, and Micell Technologies; all the remaining authors do not have any conflicts relevant to this contribution.

Provenance and peer review Not commissioned; externally peer reviewed.

Open Access This is an Open Access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 3.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: <http://creativecommons.org/licenses/by-nc/3.0/>

REFERENCES

- Greenhalgh J, Hockenhull J, Rao N, *et al.* Drug-eluting stents versus bare metal stents for angina or acute coronary syndromes. *Cochrane Database Syst Rev* 2010;(5):CD004587.
- Camenzind E, Steg PG, Wijns W. Stent thrombosis late after implantation of first-generation drug-eluting stents: a cause for concern. *Circulation* 2007;115:1440–55; discussion 1455.
- Daemen J, Wenaweser P, Tsuchida K, *et al.* Early and late coronary stent thrombosis of sirolimus-eluting and paclitaxel-eluting stents in routine clinical practice: data from a large two-institutional cohort study. *Lancet* 2007;369:667–78.
- Joner M, Finn AV, Farb A, *et al.* Pathology of drug-eluting stents in humans: delayed healing and late thrombotic risk. *J Am Coll Cardiol* 2006;48:193–202.
- Navarese EP, Tandjung K, Claessen B, *et al.* Safety and efficacy outcomes of first and second generation durable polymer drug eluting stents and biodegradable polymer biolimus eluting stents in clinical practice: comprehensive network meta-analysis. *BMJ* 2013;347:f6530.
- Sethi A, Bahekar A, Bhuriya R, *et al.* Zotarolimus-eluting stent versus sirolimus-eluting and paclitaxel-eluting stents for percutaneous coronary intervention: a meta-analysis of randomized trials. *Arch Cardiovasc Dis* 2012;105:544–56.
- Fan J, Du H, Yin Y, *et al.* Efficacy and safety of zotarolimus-eluting stents compared with sirolimus-eluting stents in patients undergoing percutaneous coronary interventions—a meta-analysis of randomized controlled trials. *Int J Cardiol* 2013;167:2126–33.
- Park KW, Kang SH, Velders MA, *et al.* Safety and efficacy of everolimus- versus sirolimus-eluting stents: a systematic review and meta-analysis of 11 randomized trials. *Am Heart J* 2013;165:241–50 e4.
- Liberati A, Altman DG, Tetzlaff J, *et al.* The PRISMA statement for reporting systematic reviews and meta-analyses of studies that evaluate health care interventions: explanation and elaboration. *Ann Intern Med* 2009;151:W65–94.
- Cutlip DE, Windecker S, Mehran R, *et al.* Clinical end points in coronary stent trials: a case for standardized definitions. *Circulation* 2007;115:2344–51.
- Higgins JP, Thompson SG, Deeks JJ, *et al.* Measuring inconsistency in meta-analyses. *BMJ* 2003;327:557–60.
- Fleiss JL. Analysis of data from multiclinic trials. *Control Clin Trials* 1986;7:267–75.
- Velders MA, Boven AJV, Hofma SH. *Xience V stent vs. Cypher stent in all-comer patients: a randomized trial.* Unpublished Work, 2012.
- Velders MA, Hofma SH, Brouwer J, *et al.* Two-year results of an open-label randomized comparison of everolimus-eluting stents and sirolimus-eluting stents. *PLoS ONE* 2013;8:e64424.
- Kaiser C, Galatius S, Erne P, *et al.* Drug-eluting versus bare-metal stents in large coronary arteries. *N Engl J Med* 2010;363:2310–19.
- Park HJ, Kim HY, Lee JM, *et al.* Randomized comparison of the efficacy and safety of zotarolimus-eluting stents vs. sirolimus-eluting stents for percutaneous coronary intervention in chronic total occlusion—CATHolic Total Occlusion Study (CATOS) trial. *Circ J* 2012;76:868–75.
- Moreno R, Garcia E, Teles R, *et al.* Randomized comparison of sirolimus-eluting and everolimus-eluting coronary stents in the treatment of total coronary occlusions: results from the chronic coronary occlusion treated by everolimus-eluting stent randomized trial. *Circ Cardiovasc Interv* 2013;6:21–8.
- Kedhi E, Joesoef KS, McFadden E, *et al.* Second-generation everolimus-eluting and paclitaxel-eluting stents in real-life practice (COMPARE): a randomised trial. *Lancet* 2010;375:201–9.
- Smits PC, Kedhi E, Roayaards KJ, *et al.* 2-year follow-up of a randomized controlled trial of everolimus- and paclitaxel-eluting stents for coronary revascularization in daily practice. COMPARE (Comparison of the everolimus eluting XIENCE-V stent with the paclitaxel eluting TAXUS LIBERTE stent in all-comers: a randomized open label trial). *J Am Coll Cardiol* 2011;58:11–18.
- <http://www.medscape.com/viewarticle/714902> (accessed Jan 2014).
- Kandzari DE, Leon MB, Popma JJ, *et al.* Comparison of zotarolimus-eluting and sirolimus eluting stents in patients with native coronary artery disease: a randomized controlled trial. *J Am Coll Cardiol* 2006;48:2440–7.
- Kandzari DE, Mauri L, Popma JJ, *et al.* Late-term clinical outcomes with zotarolimus- and sirolimus-eluting stents. 5-year follow-up of the ENDEAVOR III (A Randomized Controlled Trial of the Medtronic Endeavor Drug [ABT-578] Eluting Coronary Stent System Versus the Cypher Sirolimus-Eluting Coronary Stent System in De Novo Native Coronary Artery Lesions). *JACC Cardiovasc Interv* 2011;4:543–50.
- Leon MB, Mauri L, Popma JJ, *et al.* A randomized comparison of the Endeavor zotarolimus-eluting stent versus the TAXUS paclitaxel-eluting stent in de novo native coronary lesions 12-month outcomes from the ENDEAVOR IV trial. *J Am Coll Cardiol* 2010;55:543–54.
- Kirtane AJ, Leon MB, Ball MW, *et al.* The “final” 5-year follow-up from the ENDEAVOR IV trial comparing a zotarolimus-eluting stent with a paclitaxel-eluting stent. *JACC Cardiovasc Interv* 2013;6:325–33.
- Kim WJ, Lee SW, Park SW, *et al.* Randomized comparison of everolimus-eluting stent versus sirolimus-eluting stent implantation for de novo coronary artery disease in patients with diabetes mellitus (ESSENCE-DIABETES): results from the ESSENCE-DIABETES trial. *Circulation* 2011;124:886–92.
- Park KW, Chae IH, Lim DS, *et al.* Everolimus-eluting versus sirolimus-eluting stents in patients undergoing percutaneous coronary intervention: the EXCELLENT (Efficacy of Xience/Promus Versus Cypher to Reduce Late Loss After Stenting) randomized trial. *J Am Coll Cardiol* 2011;58:1844–54.
- Ribichini F, Romano M, Rosiello R, *et al.* A Clinical and Angiographic Study of the XIENCE V Everolimus-Eluting Coronary Stent System in the Treatment of Patients With Multivessel Coronary Artery Disease: The EXECUTIVE Trial (EXECutive RCT: Evaluating XIENCE V in a Multi Vessel Disease). *JACC Cardiovasc Interv* 2013;6:1012–22.
- Byrne RA, Mehilili J, Iijima R, *et al.* A polymer-free dual drug-eluting stent in patients with coronary artery disease: a randomized trial vs. polymer-based drug-eluting stents. *Eur Heart J* 2009;30:923–31.
- Byrne RA, Kastrati A, Tiroch K, *et al.* 2-year clinical and angiographic outcomes from a randomized trial of polymer-free dual drug-eluting stents versus polymer-based Cypher and Endeavor [corrected] drug-eluting stents. *J Am Coll Cardiol* 2010;55:2536–43.
- Kang WC, Ahn T, Lee K, *et al.* Comparison of zotarolimus-eluting stents versus sirolimus-eluting stents versus paclitaxel-eluting stents for primary percutaneous coronary intervention in patients with ST-elevation myocardial infarction: results from the Korean Multicentre Endeavor (KOMER) acute myocardial infarction (AMI) trial. *EuroIntervention* 2011;7:936–43.

31. Park DW, Kim YH, Song HG, *et al.* Comparison of everolimus- and sirolimus-eluting stents in patients with long coronary artery lesions: a randomized LONG-DES-III (Percutaneous Treatment of LONG Native Coronary Lesions With Drug-Eluting Stent-III) Trial. *JACC Cardiovasc Interv* 2011;4:1096–103.
32. Ahn JM, Park DW, Kim YH, *et al.* Comparison of resolute zotarolimus-eluting stents and sirolimus-eluting stents in patients with de novo long coronary artery lesions: a randomized LONG-DES IV trial. *Circ Cardiovasc Interv* 2012;5:633–40.
33. Briguori C, Airoldi F, Visconti G, *et al.* Novel approaches for preventing or limiting events in diabetic patients (Naples-diabetes) trial: a randomized comparison of 3 drug-eluting stents in diabetic patients. *Circ Cardiovasc Interv* 2011;4:121–9.
34. Van den Branden BJ, Teeuwen K, Koolen JJ, *et al.* Primary Stenting of Totally Occluded Native Coronary Arteries III (PRISON III): a randomised comparison of sirolimus-eluting stent implantation with zotarolimus-eluting stent implantation for the treatment of total coronary occlusions. *EuroIntervention* 2013;9:841–53.
35. Xu B, Yang Y, Yuan Z, *et al.* Zotarolimus- and paclitaxel-eluting stents in an all-comer population in China: the RESOLUTE China randomized controlled trial. *JACC Cardiovasc Interv* 2013;6:664–70.
36. Kimura T, Morimoto T, Natsuaki M, *et al.* Comparison of everolimus-eluting and sirolimus-eluting coronary stents: 1-year outcomes from the Randomized Evaluation of Sirolimus-eluting Versus Everolimus-eluting stent Trial (RESET). *Circulation* 2012;126:1225–36.
37. Sakakibara T, Ishii H, Toriyama T, *et al.* Sirolimus-eluting stent vs. everolimus-eluting stent for coronary intervention in patients on chronic hemodialysis. *Circ J* 2012;76:351–5.
38. Sawada T, Shinke T, Otake H, *et al.* Comparisons of detailed arterial healing response at seven months following implantation of an everolimus- or sirolimus-eluting stent in patients with ST-segment elevation myocardial infarction. *Int J Cardiol* 2013;168:960–6.
39. Burzotta F, Trani C, Todaro D, *et al.* Prospective randomized comparison of sirolimus- or everolimus-eluting stent to treat bifurcated lesions by provisional approach. *JACC Cardiovasc Interv* 2011;4:327–35.
40. Chung WY, Kang J, Cho YS, *et al.* A randomized, prospective, two-center comparison of sirolimus-eluting stent and zotarolimus-eluting stent in acute ST-elevation myocardial infarction: the SEZE trial. *Chin Med J* 2012;125:3373–81.
41. Song HG, Park DW, Kim YH, *et al.* Randomized trial of optimal treatment strategies for in-stent restenosis after drug-eluting stent implantation. *J Am Coll Cardiol* 2012;59:1093–100.
42. Rasmussen K, Maeng M, Kaltoft A, *et al.* Efficacy and safety of zotarolimus-eluting and sirolimus-eluting coronary stents in routine clinical care (SORT OUT III): a randomised controlled superiority trial. *Lancet* 2010;375:1090–9.
43. Maeng M, Tilsted HH, Jensen LO, *et al.* 3-Year clinical outcomes in the randomized SORT OUT III superiority trial comparing zotarolimus- and sirolimus-eluting coronary stents. *JACC Cardiovasc Interv* 2012;5:812–18.
44. Jensen LO, Thayssen P, Hansen HS, *et al.* Randomized comparison of everolimus-eluting and sirolimus-eluting stents in patients treated with percutaneous coronary intervention: the Scandinavian Organization for Randomized Trials with Clinical Outcome IV (SORT OUT IV). *Circulation* 2012;125:1246–55.
45. Jensen LO, Thayssen P, Christiansen EH, *et al.* 2-year patient-related versus stent-related outcomes: the SORT OUT IV (Scandinavian Organization for Randomized Trials With Clinical Outcome IV) Trial. *J Am Coll Cardiol* 2012;60:1140–7.
46. Serruys PW, Ruygrok P, Neuzner J, *et al.* A randomised comparison of an everolimus-eluting coronary stent with a paclitaxel-eluting coronary stent: the SPIRIT II trial. *EuroIntervention* 2006;2:286–94.
47. Onuma Y, Miquel-Hebert K, Serruys PW, *et al.* Five-year long-term clinical follow-up of the XIENCE V everolimus-eluting coronary stent system in the treatment of patients with de novo coronary artery disease: the SPIRIT II trial. *EuroIntervention* 2013;8:1047–51.
48. Stone GW, Midei M, Newman W, *et al.* Comparison of an everolimus-eluting stent and a paclitaxel-eluting stent in patients with coronary artery disease: a randomized trial. *JAMA* 2008;299:1903–13.
49. Applegate RJ, Yaqub M, Hermiller JB, *et al.* Long-term (three-year) safety and efficacy of everolimus-eluting stents compared to paclitaxel-eluting stents (from the SPIRIT III Trial). *Am J Cardiol* 2011;107:833–40.
50. Stone GW, Rizvi A, Newman W, *et al.* Everolimus-eluting versus paclitaxel-eluting stents in coronary artery disease. *N Engl J Med* 2010;362:1663–74.
51. Stone GW, Rizvi A, Sudhir K, *et al.* Randomized comparison of everolimus- and paclitaxel-eluting stents. 2-year follow-up from the SPIRIT (Clinical Evaluation of the XIENCE V Everolimus Eluting Coronary Stent System) IV trial. *J Am Coll Cardiol* 2011;58:19–25.
52. Grube E, Chevalier B, Guagliumi G, *et al.* The SPIRIT V diabetic study: a randomized clinical evaluation of the XIENCE V everolimus-eluting stent vs the TAXUS Liberte paclitaxel-eluting stent in diabetic patients with de novo coronary artery lesions. *Am Heart J* 2012;163:867–75 e1.
53. Wang L, Zhang D, Yang X, *et al.* Comparison of safety and efficacy of Cypher® stent and Endeavor® stent in patients with acute ST elevation myocardial infarction (STEMI) undergoing emergency PCI. *J Am Coll Cardiol* 2011;58:B216 (Abstract).
54. Hofma SH, Brouwer J, Velders MA, *et al.* Second-generation everolimus-eluting stents versus first-generation sirolimus-eluting stents in acute myocardial infarction. 1-year results of the randomized XAMI (XienceV Stent vs. Cypher Stent in Primary PCI for Acute Myocardial Infarction) trial. *J Am Coll Cardiol* 2012;60:381–7.
55. Park DW, Kim YH, Yun SC, *et al.* Comparison of zotarolimus-eluting stents with sirolimus- and paclitaxel-eluting stents for coronary revascularization: the ZEST (comparison of the efficacy and safety of zotarolimus-eluting stent with sirolimus-eluting and paclitaxel-eluting stent for coronary lesions) randomized trial. *J Am Coll Cardiol* 2010;56:1187–95.
56. Lee CW, Park DW, Lee SH, *et al.* Comparison of the efficacy and safety of zotarolimus-, sirolimus-, and paclitaxel-eluting stents in patients with ST-elevation myocardial infarction. *Am J Cardiol* 2009;104:1370–6.
57. [http://www.trialresultscenter.org/study8670-ZEST-AMI-\(vs-SES\).htm](http://www.trialresultscenter.org/study8670-ZEST-AMI-(vs-SES).htm); [http://www.trialresultscenter.org/study8670-ZEST-AMI-\(vs-PES\).htm](http://www.trialresultscenter.org/study8670-ZEST-AMI-(vs-PES).htm) (accessed Jan 2014).
58. Radeleff B, Lopez-Benitez R, Stampfl U, *et al.* Paclitaxel-induced arterial wall toxicity and inflammation: tissue uptake in various dose densities in a minipig model. *J Vasc Interv Radiol* 2010;21:1262–70.
59. Stampfl U, Radeleff B, Sommer C, *et al.* Paclitaxel-induced arterial wall toxicity and inflammation: part 2—long-term tissue response in a minipig model. *J Vasc Interv Radiol* 2009;20:1608–16.
60. Applegate R, Hermiller J, Williams J, *et al.* Evaluation of the effects of everolimus-eluting and paclitaxel-eluting stents on target lesions with jailed side branches: 2-year results from the SPIRIT III randomized trial. *Catheter Cardiovasc Interv* 2010;76:644–51.
61. Joner M, Nakazawa G, Finn AV, *et al.* Endothelial cell recovery between comparator polymer-based drug-eluting stents. *J Am Coll Cardiol* 2008;52:333–42.
62. Nakatani S, Nishino M, Taniike M, *et al.* Initial findings of impact of strut width on stent coverage and apposition of sirolimus-eluting stents assessed by optical coherence tomography. *Catheter Cardiovasc Interv* 2013;81:776–81.
63. Hausleiter J, Kastrati A, Mehilli J, *et al.* Impact of lesion complexity on the capacity of a trial to detect differences in stent performance: results from the ISAR-STREO trial. *Am Heart J* 2003;146:882–6.
64. Nakazawa G, Finn AV, John MC, *et al.* The significance of preclinical evaluation of sirolimus-, paclitaxel-, and zotarolimus-eluting stents. *Am J Cardiol* 2007;100:36M–44M.
65. Silber S, Windecker S, Vranckx P, *et al.* Unrestricted randomised use of two new generation drug-eluting coronary stents: 2-year patient-related versus stent-related outcomes from the RESOLUTE All Comers trial. *Lancet* 2011;377:1241–7.

First-generation versus second-generation drug-eluting stents in current clinical practice: updated evidence from a comprehensive meta-analysis of randomised clinical trials comprising 31 379 patients

Eliano Pio Navarese, Mariusz Kowalewski, David Kandzari, Alexandra Lansky, Bartosz Górny, Lukasz Koltowski, Ron Waksman, Sergio Berti, Giuseppe Musumeci, Ugo Limbruno, Rene J van der Schaaf, Malte Kelm, Jacek Kubica and Harry Suryapranata

Open Heart 2014 1:
doi: 10.1136/openhrt-2014-000064

Updated information and services can be found at:
<http://openheart.bmj.com/content/1/1/e000064>

These include:

- | | |
|-------------------------------|--|
| Supplementary Material | Supplementary material can be found at:
http://openheart.bmj.com/content/suppl/2014/08/21/1.1.e000064.DC1.html |
| References | This article cites 62 articles, 11 of which you can access for free at:
http://openheart.bmj.com/content/1/1/e000064#BIBL |
| Open Access | This is an Open Access article distributed in accordance with the Creative Commons Attribution Non Commercial (CC BY-NC 3.0) license, which permits others to distribute, remix, adapt, build upon this work non-commercially, and license their derivative works on different terms, provided the original work is properly cited and the use is non-commercial. See: http://creativecommons.org/licenses/by-nc/3.0/ |
| Email alerting service | Receive free email alerts when new articles cite this article. Sign up in the box at the top right corner of the online article. |
-

Notes

To request permissions go to:
<http://group.bmj.com/group/rights-licensing/permissions>

To order reprints go to:
<http://journals.bmj.com/cgi/reprintform>

To subscribe to BMJ go to:
<http://group.bmj.com/subscribe/>