

## PDF hosted at the Radboud Repository of the Radboud University Nijmegen

The following full text is a publisher's version.

For additional information about this publication click this link.

<https://hdl.handle.net/2066/220793>

Please be advised that this information was generated on 2020-11-25 and may be subject to change.

# Improvement of image quality on low-dose dynamic myocardial perfusion computed tomography with a novel 4-dimensional similarity filter

Satonori Tsuneta, MD<sup>a,c</sup> , Noriko Oyama-Manabe, MD, PhD<sup>b,\*</sup>, Hiroyuki Kameda, MD, PhD<sup>d</sup>, Taisuke Harada, MD, PhD<sup>a</sup>, Fumi Kato, MD, PhD<sup>a</sup>, Ewoud J. Smit, MD, PhD<sup>e</sup>, Mathias Prokop, MD, PhD<sup>e</sup>, Kohsuke Kudo, MD, PhD<sup>c</sup>

## Abstract

The aim of this study was to evaluate the effect of a novel 4-dimensional similarity filter (4DSF) on quantitative and qualitative parameters of low-dose dynamic myocardial computed tomography perfusion (CTP) images.

In this retrospective study, medical records of 32 patients with suspected or known coronary artery disease who underwent dynamic myocardial CTP at 80 kV were included. The 4DSF reduces noise by averaging voxels that have similar dynamic behavior after adaptive iterative dose reduction 3D (AIDR3D) and deformable image registration were applied. Qualitative (artefact, contour sharpness, and myocardial homogeneity [1 = poor; 2 = intermediate; 3 = good]) and quantitative measurement (standard deviation [SD] and signal-to-noise ratio [SNR]) were compared between the 4DSF and AIDR3D. Contrast-to-noise ratio (CNR) between ischemic and normal remote myocardium was also assessed using myocardial perfusion magnetic resonance imaging as the reference standard in seven patients.

The 4DSF was successfully applied to all the images. Improvement in subjective image quality yielded by 4DSF was higher than that yielded by AIDR3D (homogeneity, 1.0 [3 vs 2]; artefact, 1.5 [3 vs 1.5];  $P < .001$ ) in all patients. The 4DSF significantly decreased the SD by 59% (AIDR3D vs 4DSF:  $33.5 \pm 0.4$  vs  $13.8 \pm 0.4$ ,  $P < .001$ ), increased the SNR by 134% (AIDR3D vs 4DSF:  $4.4 \pm 0.2$  vs  $10.3 \pm 0.2$ ,  $P < .001$ ), and increased the CNR by 131% (AIDR3D vs 4DSF:  $1.6 \pm 0.2$  vs  $3.7 \pm 0.2$ ,  $P < .001$ ).

The 4DSF improved the qualitative and quantitative parameters of low-dose dynamic myocardial CTP images.

**Abbreviations:** 4DSF = 4-dimensional similarity filter, AIDR3D = adaptive iterative dose reduction 3D, ATP = adenosine triphosphate, CNR = contrast-to-noise ratio, CTP = computed tomography perfusion, ECG = electrocardiography, HU = Hounsfield unit, IQR = interquartile range, LV = left ventricle, MDCT = multi-detector row computed tomography, MRI = magnetic resonance imaging, ROI = region of interest, SD = standard deviation, SNR = signal-to-noise ratio.

**Keywords:** dynamic myocardial computed tomography perfusion, four-dimensional similarity filter, ischaemic heart disease, noise reduction technique

## 1. Introduction

Myocardial computed tomography perfusion (CTP) with coronary CT angiography as a single modality can help diagnose functional myocardial ischemia in addition to coronary anatomical stenosis.<sup>[1]</sup> Compared to static CTP, dynamic CTP has more

advantages, such as quantitative evaluation of absolute myocardial blood flow and coronary flow reserve and ability to capture the peak myocardial enhancement.<sup>[2]</sup> However, dynamic CTP is associated with a higher radiation dose. To solve this problem, dynamic low-dose CTP has been used.<sup>[3]</sup> However, the image noise would be increased at low dose.<sup>[3]</sup> Recently, iterative

Editor: Ismaheel Lawal.

The authors report no conflicts of interest.

The datasets generated during and/or analyzed during the current study are available from the corresponding author on reasonable request.

<sup>a</sup> Department of Diagnostic and Interventional Radiology, Hokkaido University Hospital, Sapporo, Hokkaido, <sup>b</sup> Department of Radiology, Saitama Medical Center, Jichi Medical University, Saitama-shi, Saitama, <sup>c</sup> Department of Diagnostic Imaging, Hokkaido University Graduate School of Medicine, Sapporo, Hokkaido, <sup>d</sup> Department of Dental Radiology, Hokkaido University Graduate School of Dental Medicine, Sapporo, Hokkaido, Japan, <sup>e</sup> Department of Radiology and Nuclear Medicine, Radboud University Medical Center, Nijmegen, The Netherlands.

\* Correspondence: Noriko Oyama-Manabe, Department of Radiology, Saitama Medical Center, Jichi Medical University, 1-847, Amanumacho, Omiya-ku, Saitama-shi, Saitama 330-8503, Japan (e-mail: norikomanabe@jichi.ac.jp).

Copyright © 2020 the Author(s). Published by Wolters Kluwer Health, Inc.

This is an open access article distributed under the terms of the Creative Commons Attribution-Non Commercial License 4.0 (CCBY-NC), where it is permissible to download, share, remix, transform, and buildup the work provided it is properly cited. The work cannot be used commercially without permission from the journal.

How to cite this article: Tsuneta S, Oyama-Manabe N, Kameda H, Harada T, Kato F, Smit EJ, Prokop M, Kudo K. Improvement of image quality on low-dose dynamic myocardial perfusion computed tomography with a novel four-dimensional similarity filter. *Medicine* 2020;99:26(e20804).

Received: 9 March 2020 / Received in final form: 20 May 2020 / Accepted: 21 May 2020

<http://dx.doi.org/10.1097/MD.00000000000020804>

reconstruction methods such as adaptive iterative dose reduction 3D (AIDR3D; Canon Medical Systems, Otawara, Japan) have been adapted for noise reduction in dynamic CTP.<sup>[4–6]</sup> However, iterative reconstruction works for only spatial domain.

Although there were a few studies focusing on noise reduction method for dynamic CTP that works for the time domain,<sup>[7,8]</sup> most of these methods simply averaged temporally neighboring series. We applied a newly developed 4-dimensional similarity filter (4DSF), which uses per voxel-similarity within the 4D acquisition sequence to average identically perfused tissues, that is, showing similar time density curves to reduce image noise.

The purpose of this study was to compare the effects of the 4DSF and AIDR3D on quantitative and qualitative parameters of low-dose dynamic myocardial CTP image.

## 2. Methods

### 2.1. Patients

This was a retrospective and single-center study (Hokkaido University Hospital). Ethical approval was obtained from our institutional review board. The requirement for informed consent was waived because of the retrospective nature of the study. Thirty-five patients with confirmed or suspected coronary artery disease who underwent dynamic myocardial CTP at 80 kV from April 2015 to March 2017 were enrolled; patient inclusion and exclusion and patient preparation were performed as reported previously.<sup>[9]</sup> We excluded 3 patients who previously underwent coronary artery bypass grafting. Therefore, medical records of 32 patients were finally evaluated (aged  $67.7 \pm 7.5$  years). The patient characteristics are summarized in Table 1.

### 2.2. CT examination protocol

All patients were scanned with 320-row MDCT (Aquilion ONE VISION edition; Canon Medical Systems Corporation, Otawara, Japan). Dynamic CTP was performed with a tube potential of 80 kV, tube current of 120 mA at 75% R-R interval, and a rotation time of 0.275 seconds.

The protocols of CTP have been previously reported in detail.<sup>[9]</sup> In brief, with a continuous 6-minute infusion of adenosine triphosphate (ATP; 0.16 mg/kg/min), stress dynamic CTP imaging was performed for 25 seconds with 50 mL of an iodinated contrast agent (Iohexol, 350 mgI/mL, Daiichi Sankyo,

Tokyo, Japan) and 30 mL of saline chaser (5.0 mL/s). After a 15-minute interval, rest CTP was performed in the same way as stress dynamic CTP was performed.

Reconstruction was performed at 1-mm intervals using AIDR3D at strong level and beam-hardening correction as the standard dataset.

### 2.3. Four-dimensional similarity filter

A dynamic myocardial computed tomography perfusion (CTP) dataset has a vast number of voxels. Each voxel has CT values which changes along time. Since 4DSF is particularly useful for spatially consistent data, motion compensation should be applied to create a dataset that is consistent beforehand. 4DSF needs a large number of voxels having a similar dynamic behavior.  $x$  and  $y$  are defined as voxel locations within the datasets. The number of phases is defined as  $m$  and the sampled phase is defined as  $i$ .  $I(x, i)$  is original CT value of a voxel.  $Ii(x)$  is CT value vector at location  $x$  excluding phase  $i$ :

$$Ii(x) = (I(x, 1), I(x, 2), \dots, I(x, i-1), I(x, i+1), \dots, I(x, m)).$$

$D(Ii(x), Ii(y))$  is a distance between vectors  $Ii(x)$  and  $Ii(y)$ :

$$D(Ii(x), Ii(y)) = \sqrt{\sum_{j=1, j \neq i}^m [Ij(y) - Ij(x)]^2}$$

4DSF searches the suitable voxel  $I(y, i)$  to make  $D(Ii(x), Ii(y))$  the smallest throughout the whole 3-dimensional datasets, and then replace  $I(x, i)$  and  $I(y, i)$ . 4DSF repeats this process over and over and make the time-intensity curves smoother. The global search for similar voxels provides a more natural texture than local spatial filtering does. In addition, this method reduces motion artefacts and provides extremely stable images of anatomic structures across the whole dynamic acquisition. Because filtering mainly occurs in the temporal domain, spatial resolution is not reduced and the sharpness of tissue contour is preserved.<sup>[10]</sup>

4DSF can be applied by the specific software with these algorithm installed in the commercially available workstation (Vitrea; Canon Medical Systems Corporation, Otawara, Japan). 4DSF can be applied to each stress and rest CTP dataset, respectively.

In this study, 4DSF was additionally applied to the standard dynamic datasets with AIDR3D, which was applied to each of stress and rest dynamic 3D volume datasets. Deformable image registration was performed with Vitrea workstation before applying 4DSF.

### 2.4. Myocardial perfusion MRI acquisition

Presence of myocardial ischemia was evaluated in 7 patients by myocardial perfusion MRI. All seven patients had myocardial ischemia with multivessel diseases.

Perfusion MRI was performed using a 3T whole-body scanner (Achieva Tx; Philips Medical Systems, Best, The Netherlands) with a 32-channel phased-array receiver torso-cardiac coil. The turbo field-echo technique with saturation recovery magnetization (slice thickness, 8 mm; field of view, 380 mm × 380 mm; matrix, 224 × 224) was used.

Stress myocardial perfusion MRI was performed as described previously.<sup>[11]</sup> In brief, perfusion MR images were obtained using ECG-triggered breath-hold technique in three short axes (basal, mid-ventricular, and apical). Three minutes after ATP infusion

**Table 1**

#### Patient characteristics.

No. of patients	32
Age	$67.7 \pm 7.5$
Male sex, n (%)	18 (56)
Height, cm	$160.6 \pm 8.3$
Body weight, kg	64.3 (53.9–71.0)
Body mass index	$25.1 \pm 3.6$
Hypertension, n (%)	24 (75)
Hyperlipidemia, n (%)	20 (63)
Diabetes mellitus, n (%)	13 (40)
Current smoker, n (%)	8 (25)
History of myocardial infarction, n (%)	1 (3)
History of percutaneous catheter intervention, n (%)	5 (16)

Age, sex, and body mass index are expressed as mean  $\pm$  SD. Body weight is expressed as median (interquartile range). The remaining parameters were expressed as the number of patients (percentage).

(0.16 mg/kg/min), dynamic stress myocardial perfusion MRI was performed with 0.03 mmol/kg Gd-DTPA (Magnevist, Bayer, Wayne, NJ) and 20 mL saline chaser (4.0 mL/s). Rest myocardial perfusion MRI was also performed after stress myocardial perfusion MRI.

### 2.5. Qualitative analysis

The images were reformatted with short axes of the left ventricle (LV) at the basal, mid, and apical levels for each of the stress and rest CTP images at the peak enhancement of myocardium, with a slice thickness of 3 mm. Two independent readers (HK and TH; board certified radiologists) evaluated the image quality in a blinded, randomized fashion. They took a training course how to interpret dynamic myocardial CTP before the evaluation (the lecture about anatomy and image interpretation of dynamic CTP, and hands-on session using six datasets [stress and rest images] with three vessel territories for each basal, mid-ventricular and apical slice). Visual quality of each AIDR3D and 4DSF image belonging to the 32 patients was subjectively graded (artefacts for stress and rest, contour sharpness between LV cavity and myocardium, and myocardial homogeneity for rest images) for each of the 3 coronary territories on a 3-point scale (1=poor, 2=intermediate, 3=good). Per-patient scores of the three vessel territories were averaged. The grades were averaged between readers for each measurement and patient. Inter-reader agreement was computed using kappa statistics.

### 2.6. Quantitative analysis

A radiologist (ST; 2 years of cardiac MRI experience) quantitatively assessed image quality using rest and stress images by measuring the image noise, signal-to-noise ratio (SNR), and contrast-to-noise ratio (CNR) between normal and ischemic myocardium (Fig. 1).


Regions of interest (ROI) were manually placed at each of the American Heart Association's (AHA) standard 16 myocardial segments (except for the apex) in each level (six 100 mm<sup>2</sup> ROIs at each basal and mid-ventricular segment, and 4 ROIs at apical segment) at the time of peak enhancement of the myocardium. SNR was evaluated using all 16 ROIs in rest CTP images and using ROIs without visible ischemia in stress CTP images. SNR was calculated as the mean attenuation of the normal myocardium divided by the SD value.

In segments with visible ischemia, as determined by stress perfusion MRI, CNR was calculated as the difference in CT attenuation between the hypoperfused and remote myocardium, divided by the SD value of the remote myocardium.


Among the 14 myocardial datasets (7 datasets each for stress and rest CTP), 1 stress dataset was excluded because of excessive motion artefacts, and a total of 6 segments were excluded owing to beam-hardening or streak artefacts. Therefore, a total of 202 segments were included. The image noise was assessed with 154 segments (110 segments in rest CTP datasets and 44 segments in stress CTP datasets). CNR was assessed with 48 segments in stress CTP datasets. The number of patients and segments in MRI datasets are summarized in Fig. 2.

### 2.7. Statistical analysis

All data are expressed as mean  $\pm$  SD except for body weight. Because body weight was not normally distributed, it is expressed as median and interquartile range (IQR). Normal distribution was assessed using the Shapiro-Wilk test. Qualitative scores were statistically compared using the paired Wilcoxon rank sum test. Kappa statistics were computed to assess inter-reader agreement in the qualitative scores. Quantitative value was statistically assessed with Student *t* test. All statistical analyses were performed using JMP14. Differences were considered to be statistically significant when *P* values were  $<.05$ .

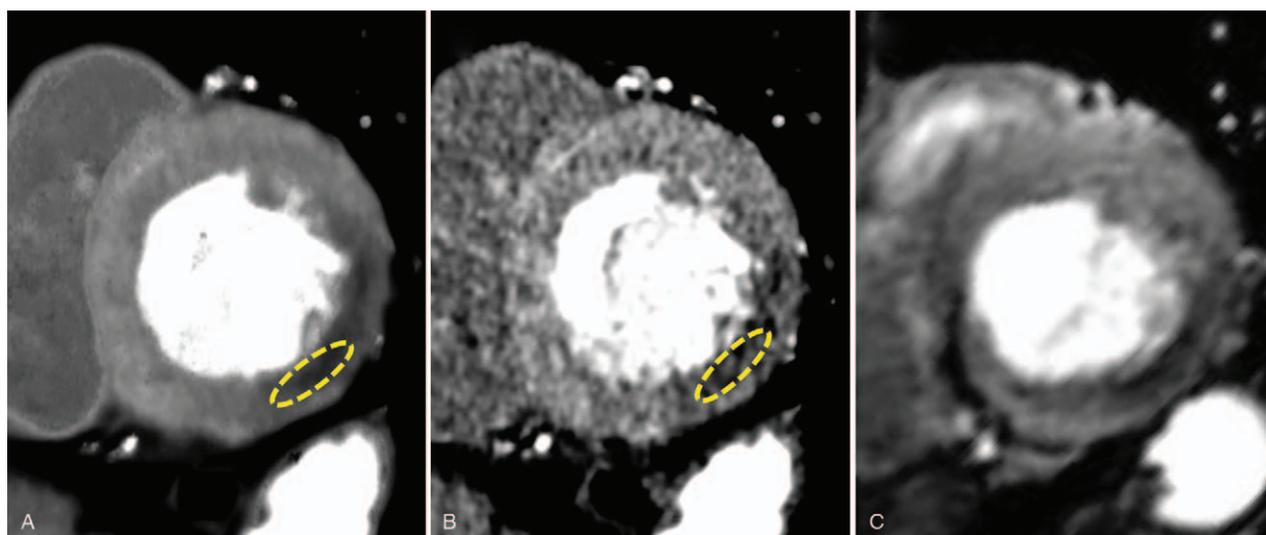

**Figure 1.** A case of a man in his 70s with severe stenosis in the left circumflex artery. The clarity of ischemia at the lateral wall in the basal level is higher with 4-dimensional similarity filter (4DSF) (A) than with adaptive iterative dose reduction 3D (AIDR3D) (B), because of less image noise; corresponding stress myocardial perfusion MR image (C) for reference. For example, the region of interest in the American Heart Association segment 5 is placed as shown in (A, B) for the calculation of contrast-to-noise ratio. In this case, visual image quality scores (artefacts, contour sharpness, myocardial homogeneity) of 4DSF were (3, 3, 3) (A) and the scores of AIDR3D were (2, 3, 2) (B).

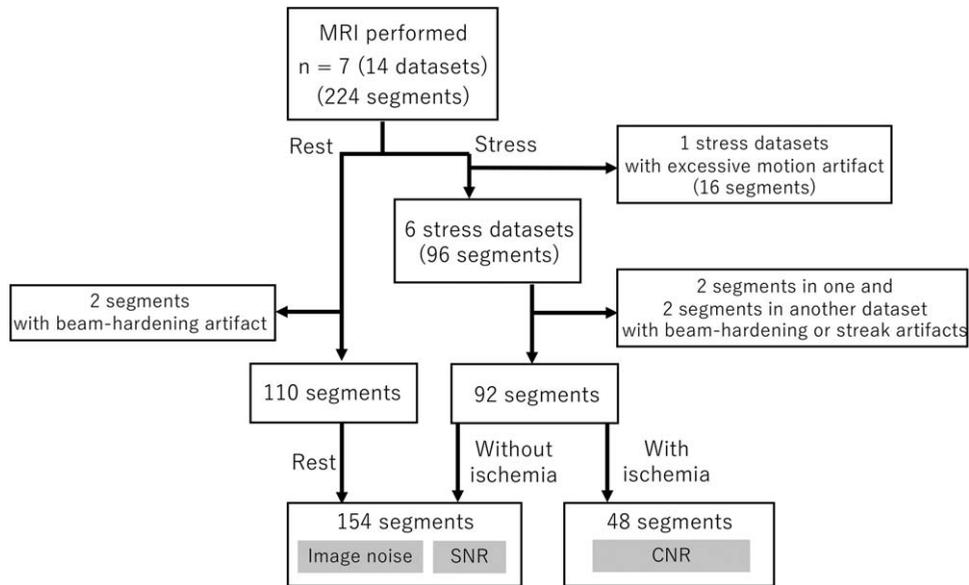

**Figure 2.** Enrolment of magnetic resonance imaging datasets. CNR = contrast-to-noise ratio, SNR = signal-to-noise ratio.

### 3. Results

The 4DSF was successfully applied to the CTP images of all 32 patients. There were no specific artefacts or technical errors in process.

#### 3.1. Qualitative analysis


There were no significant differences in the scores among the 3 coronary vessel territories. Improvement in subjective image quality yielded by using 4DSF was higher than that yielded by using AIDR3D (homogeneity, 1.0 (3.0 vs 2.0); artefacts, 1.5 (3.0 vs 1.5);  $P < .001$ ) in all images. Sharpness score was either equal or improved in all images (Fig. 3). The kappa value was moderate ( $\text{kappa} = 0.54$  [95% confidence interval, CI: 0.48–0.59]).

#### 3.2. Quantitative analysis


The 4DSF significantly decreased the mean image noise in all segments by 59% (4DSF vs AIDR3D:  $13.8 \pm 0.4$  vs  $33.5 \pm 0.4$ ,  $P < .001$ ) and increased the SNR by 134% (4DSF vs AIDR3D:  $10.3 \pm 0.2$  vs  $4.4 \pm 0.2$ ,  $P < .001$ ). The difference in CT values between normal and ischemic myocardium was  $51.8 \pm 21.0$  HU with 4DSF and  $52.2 \pm 24.4$  HU with AIDR3D. The 4DSF increased the CNR by 131% (4DSF vs AIDR3D:  $3.7 \pm 0.2$  vs  $1.6 \pm 0.2$ ,  $P < .001$ ) (Fig. 4).

### 4. Discussion

Our study applied the novel 4DSF method to low-dose dynamic myocardial CTP images. The 4DSF improved visual homogeneity

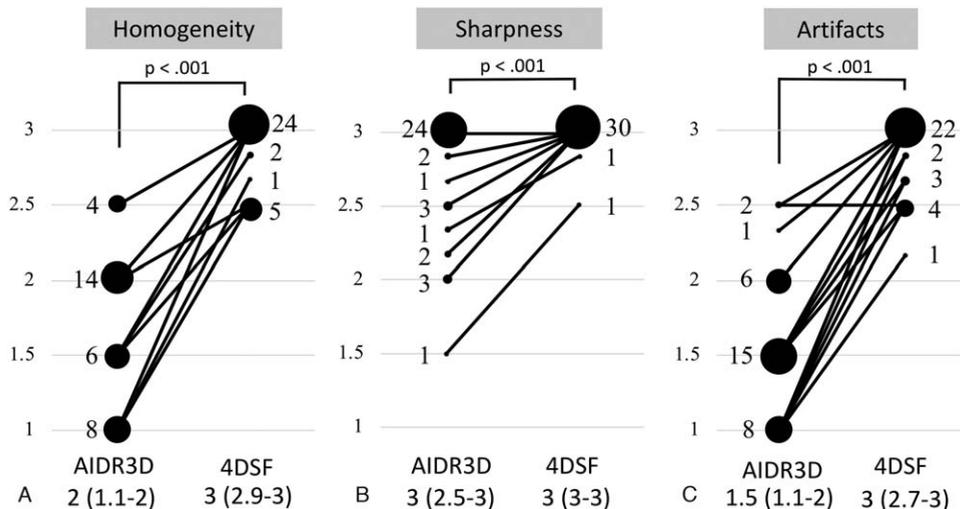

**Figure 3.** Paired plots of qualitative scores. The numbers of patients are indicated beside the dots. The dots' sizes correlate with the number of patients. The 4DSF significantly improved homogeneity and artefact scores (all,  $P < .001$ ), relative to AIDR3D (A, C). The average of sharpness score was equal but statistically improved ( $P < .001$ ) between 2 reconstructions (B). The scores were expressed as median (IQR). 4DSF = 4-dimensional similarity filter, AIDR3D = adaptive iterative dose reduction 3D.

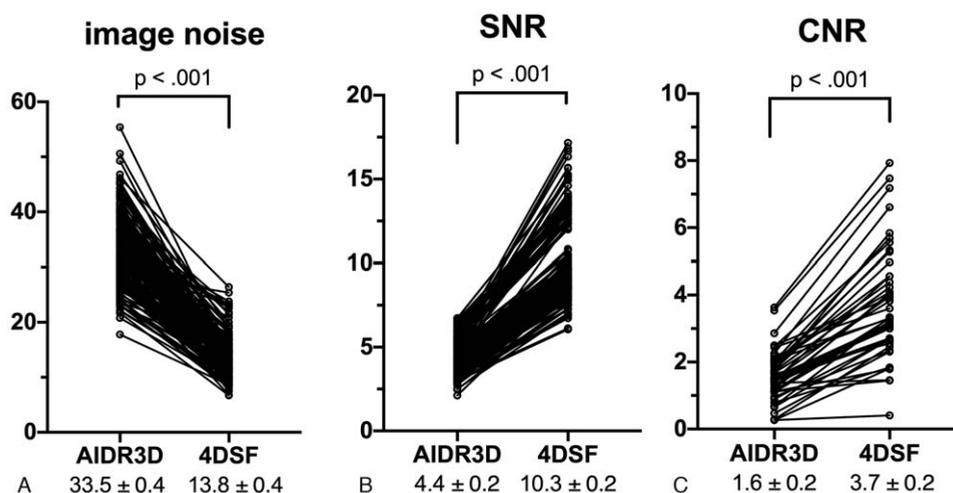

**Figure 4.** The paired comparison plots of image noise, SNR, and CNR. The mean image noise with the 4DSF was significantly lower than that with AIDR3D ( $P < .001$ ) (A). SNR with the 4DSF was significantly higher than that with AIDR3D ( $P < .001$ ) (B). CNR with the 4DSF was significantly higher than that with AIDR3D ( $P < .001$ ) (C). The scores were expressed as mean  $\pm$  SD. 4DSF = 4-dimensional similarity filter, AIDR3D = adaptive iterative dose reduction 3D, CNR = contrast-to-noise ratio, SNR = signal-to-noise ratio.

of myocardial attenuation and reduced artefacts in dynamic CTP images. Moreover, the 4DSF significantly decreased the mean image noise and increased SNR and CNR.

Myocardial CTP images have a poorer CNR than MR perfusion images do.<sup>[12]</sup> The difference in CT value between ischemic and normal remote myocardium is small, (approximately 20 HU at 100 kV).<sup>[13,14]</sup> In our study, the difference in CT value between ischemic and normal myocardium, obtained by using both the methods, was relatively high (AIDR3D, 53.6 HU; 4DSF, 51.1 HU) owing to low-dose protocol with 80 kV. Moreover, our study showed the 4DSF decreased image noise by 59% and increased CNR by 131% (4DSF vs AIDR3D: 33.5 vs 13.8 and 3.7 vs 1.6, respectively). Therefore, the 4DSF would facilitate better visualization of ischemia. Regarding subjective evaluation, myocardial homogeneity, contour sharpness, and artefacts were improved by the 4DSF.

For dynamic CTP, there were several techniques to reduce image noise, which were divided into the approaches to improve sinogram data or to improve reconstructed CT images using various filters. Iterative reconstruction technologies such as AIDR3D improve sinogram data and were generally used for noise reduction in dynamic myocardial CTP images.<sup>[5]</sup> It is effective for spatial denoising. However, it does not ensure temporal smoothness. On the other hands, noise reduction filters used for spatial denoising and temporal smoothness. Some previously reported noise reduction methods, regarding temporal domain, used temporal information to average voxels in the temporally neighbor series alone.<sup>[7,8,15]</sup> A modified simple linear iterative clustering algorithm with robust perfusion quantification (SLICR) employed temporal voxels' similarity of dynamic myocardial CTP.<sup>[16]</sup> SLICR generates super-voxels of tissues with similar hemodynamic properties on the basis of both spatial and temporal feature distances from the targeted voxel. Although SLICR is useful for calculating quantitative myocardial blood flow (MBF) or generating MBF map, generating super-voxel with SLICR leads to loss of spatial resolution. The 4DSF is unique voxel-wise algorithm that results in potent noise reduction without losing spatial resolution or temporal information. Another voxel-wise technique for high resolution myocardial

CTP has been presented that combines temporal filtering with principle component analysis.<sup>[17]</sup> In their study, image noise was reduced by 34% (SD: 21.4 vs 14.1) and SNR was increased by 47% (3.6 vs 5.3).<sup>[17]</sup> We did not compare these methods and 4DSF directly; however, their results were similar to our study. For dynamic CTP, the algorithm with temporal domain would be effective for image noise reduction.

Our study had several limitations. First, we included a small number of patients who were confirmed to have myocardial ischemia with MRI, which allowed the presentation of descriptive statistics alone. Second, this study did not compare the absolute MBF between AIDR3D and the 4DSF. We have previously established the algorithm and validated the absolute MBF values with AIDR3D compared to <sup>15</sup>O-water PET.<sup>[9,18]</sup> Since 4DSF reduced image noise, it would be expected to improve the algorithm. Further investigations must be performed to study the effect of 4DSF on the absolute myocardial blood flow.

In conclusion, the 4DSF improved the qualitative and quantitative parameters of low-dose dynamic myocardial CTP. The improvement in CNR suggests that 4DSF facilitates better visualization of myocardial ischemia in dynamic myocardial CTP images.

#### Author contributions

**Conceptualization:** Noriko Oyama-Manabe.

**Data curation:** Satonori Tsuneta.

**Formal analysis:** Satonori Tsuneta.

**Funding acquisition:** Noriko Oyama-Manabe.

**Investigation:** Satonori Tsuneta, Hiroyuki Kameda, Taisuke Harada.

**Methodology:** Noriko Oyama-Manabe, Ewoud J Smit, Mathias Prokop.

**Project administration:** Noriko Oyama-Manabe, Fumi Kato.

**Resources:** Ewoud J Smit, Mathias Prokop.

**Software:** Ewoud J Smit, Mathias Prokop.

**Supervision:** Noriko Oyama-Manabe, Kohsuke Kudo.

**Validation:** Noriko Oyama-Manabe.

**Visualization:** Satonori Tsuneta.

**Writing – original draft:** Satonori Tsuneta, Noriko Oyama-Manabe.

**Writing – review & editing:** Noriko Oyama-Manabe.

## References

- [1] Rochitte CE, George RT, Chen MY, et al. Computed tomography angiography and perfusion to assess coronary artery stenosis causing perfusion defects by single photon emission computed tomography: the CORE320 study. *Eur Heart J* 2013;35:1120–30.
- [2] Danad I, Szymonifka J, Schulman-Marcus J, et al. Static and dynamic assessment of myocardial perfusion by computed tomography. *Eur Heart J Cardiovasc Imaging* 2016;17:836–44.
- [3] Fujita M, Kitagawa K, Ito T, et al. Dose reduction in dynamic CT stress myocardial perfusion imaging: comparison of 80-kV/370-mAs and 100-kV/300-mAs protocols. *Eur Radiol* 2014;24:748–55.
- [4] Eck B, Fahmi R, Fuqua C, et al. Low dose dynamic myocardial CT perfusion using advanced iterative reconstruction. *Proc SPIE Int Soc Opt Eng* 2015;doi:10.1117/12.2081418.
- [5] Gramer BM, Muenzel D, Leber V, et al. Impact of iterative reconstruction on CNR and SNR in dynamic myocardial perfusion imaging in an animal model. *Eur Radiol* 2012;22:2654–61.
- [6] Tao Y, Chen G-H, Hacker TA, et al. Low dose dynamic CT myocardial perfusion imaging using a statistical iterative reconstruction method. *Med Phys* 2014;41:71914.
- [7] Muenzel D, Kabus S, Gramer B, et al. Perfusion imaging of the myocardium: a technical note on improvement of image quality. *PLoS One* 2013;8:e75263https://doi.org/10.1371/journal.pone.0075263.
- [8] Feger S, Shaban A, Lukas S, et al. Temporal averaging for analysis of four-dimensional whole-heart computed tomography perfusion of the myocardium: proof-of-concept study. *Int J Cardiovasc Imaging* 2017;33:371–82.
- [9] Kikuchi Y, Oyama-Manabe N, Naya M, et al. Quantification of myocardial blood flow using dynamic 320-row multi-detector CT as compared with (1)(5)O-H(2)O PET. *Eur Radiol* 2014;24:1547–56.
- [10] Smit E, Murayama K, Galen T, et al. ECR 2019: book of abstracts. *Insights Imaging* 2019;10:22.
- [11] Tomiyama Y, Manabe O, Oyama-Manabe N, et al. Quantification of myocardial blood flow with dynamic perfusion 3.0 Tesla MRI: validation with 15o-water PET. *J Magn Reson Imaging* 2015;42:754–62.
- [12] Otton J, Morton G, Schuster A, et al. A direct comparison of the sensitivity of CT and MR cardiac perfusion using a myocardial perfusion phantom. *J Cardiovasc Comput Tomogr* 2013;7:117–24.
- [13] Pelgrim GJ, Nieuwenhuis ER, Duguay TM, et al. Optimal timing of image acquisition for arterial first pass CT myocardial perfusion imaging. *Eur J Radiol* 2017;86:227–33.
- [14] Bischoff B, Bamberg F, Marcus R, et al. Optimal timing for first-pass stress CT myocardial perfusion imaging. *Int J Cardiovasc Imaging* 2013;29:435–42.
- [15] Speidel MA, Bateman CL, Tao Y, et al. Reduction of image noise in low tube current dynamic CT myocardial perfusion imaging using HYPR processing: a time-attenuation curve analysis. *Med Phys* 2013;40:11904.
- [16] Wu H, Eck BL, Levi J, et al. SLICR super-voxel algorithm for fast, robust quantification of myocardial blood flow by dynamic computed tomography myocardial perfusion imaging. *J Med imaging (Bellingham, Wash)* 2019;6:46001.
- [17] Lukas S, Feger S, Rief M, et al. Noise reduction and motion elimination in low-dose 4D myocardial computed tomography perfusion (CTP): preliminary clinical evaluation of the ASTRA4D algorithm. *Eur Radiol* 2019;29:4572–82.
- [18] Obara M, Naya M, Oyama-Manabe N, et al. Diagnostic value of quantitative coronary flow reserve and myocardial blood flow estimated by dynamic 320 MDCT scanning in patients with obstructive coronary artery disease. *Med (United States)* 2018;97: doi:10.1097/MD.00000000000011354.